

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056844.D
 Acq On : 6 Mar 2023 16:44
 Operator : CG/JU
 Sample : 01712-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZY0

Quant Time: Mar 06 17:33:38 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.421	152	17893	20.000	ng/ul	0.00
20) Naphthalene-d8	11.253	136	76303	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.019	164	56231	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.757	188	127390	20.000	ng/ul	0.00
79) Chrysene-d12	22.064	240	108061	20.000	ng/ul	0.00
88) Perylene-d12	25.595	264	115469	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.703	96	1669	5.174	ng/uL	0.00
4) Pyridine-d5	4.138	84	34977	26.865	ng/ul	0.00
7) Phenol-d5	7.545	99	54415	30.390	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.722	67	34857	31.914	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	36488	30.686	ng/ul	0.00
15) 4-Methylphenol-d8	9.108	113	42662	31.183	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	21382	33.438	ng/ul	0.00
24) 2-Nitrophenol-d4	10.324	143	25258	33.183	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.859	165	48524	33.839	ng/ul	0.00
31) 4-Chloroaniline-d4	11.376	131	55470	29.658	ng/ul	0.00
46) Dimethylphthalate-d6	14.408	166	157987	34.823	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	185336	35.943	ng/ul	0.00
54) 4-Nitrophenol-d4	15.178	143	21425	27.391	ng/ul	0.00
60) Fluorene-d10	16.006	176	145353	34.635	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.106	200	22269	26.129	ng/ul	0.00
73) Anthracene-d10	17.851	188	222641	36.025	ng/ul	0.00
81) Pyrene-d10	20.113	212	250893	34.311	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.348	264	228260	36.624	ng/ul	0.00
Target Compounds						
					Qvalue	
17) N-Nitroso-di-n-propyla...	9.108	70	1397	1.039	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056844.D
Acq On : 6 Mar 2023 16:44
Operator : CG/JU
Sample : 01712-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZY0

Quant Time: Mar 06 17:33:38 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

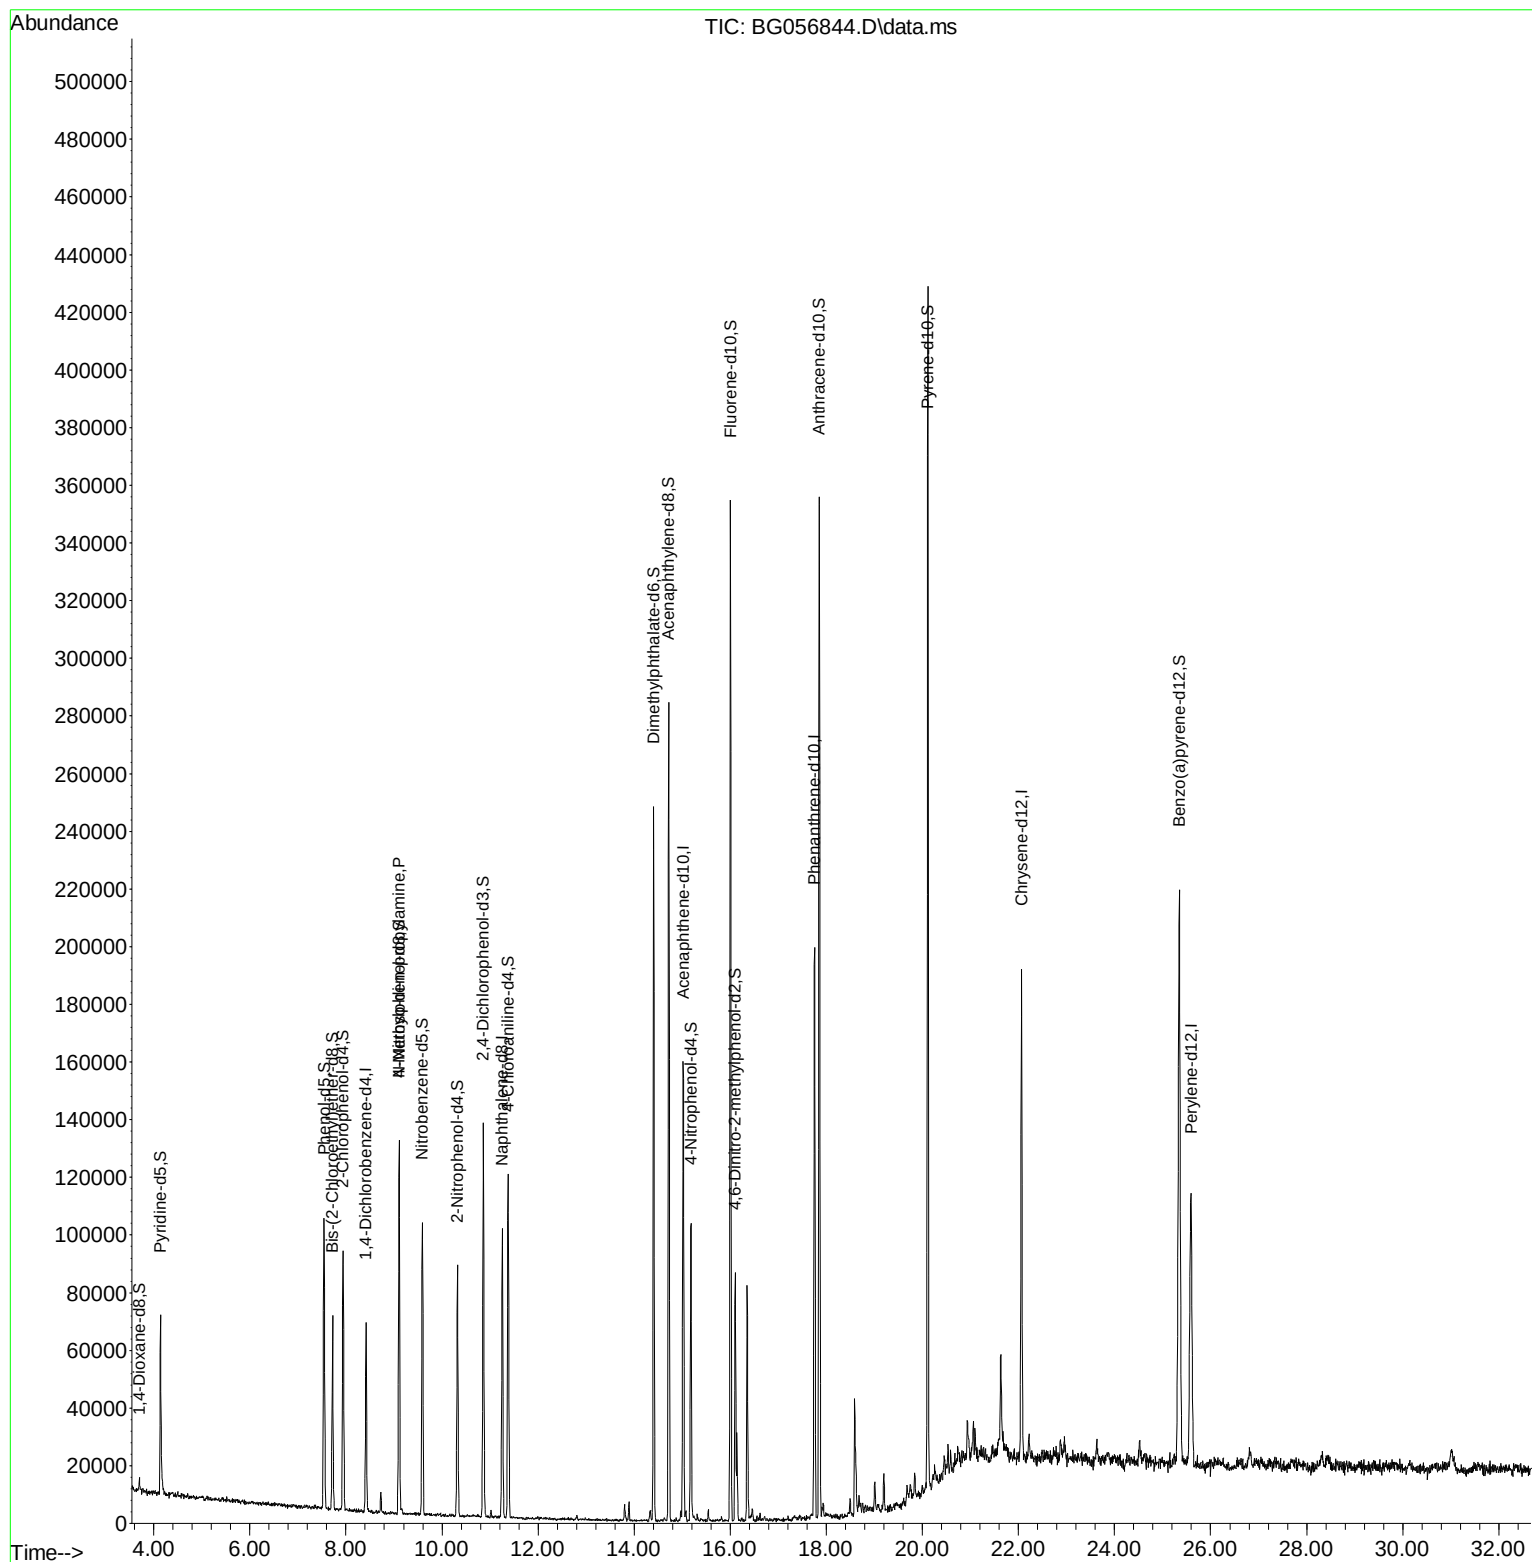

Abundance Scan 965 (9.210 min): BG056835.D\data.ms (-960) 17

N-Nitroso-di-n-propylamine

Concen: 1.039 ng/ul

RT: 9.108 min Scan#

Delta R.T. -0.108 min

Lab File: BG056844.D


Acq: 6 Mar 2023 16:44

Instrument :

BNA_G

ClientSampleId :

DBZY0

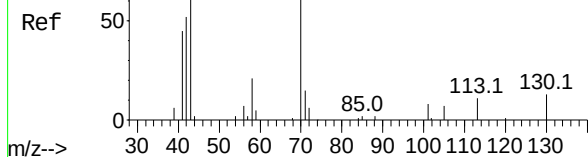

Tgt Ion: 70 Resp: 1397

Ion Ratio Lower Upper

70 100

42 297.1 46.6 70.0#

101 0.0 7.3 10.9#

130 0.0 13.7 20.5#

