




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056842.D
Acq On : 6 Mar 2023 15:21
Operator : CG/JU
Sample : 01712-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX6

Manual IntegrationsAPPROVED

Quant Time: Mar 06 16:18:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

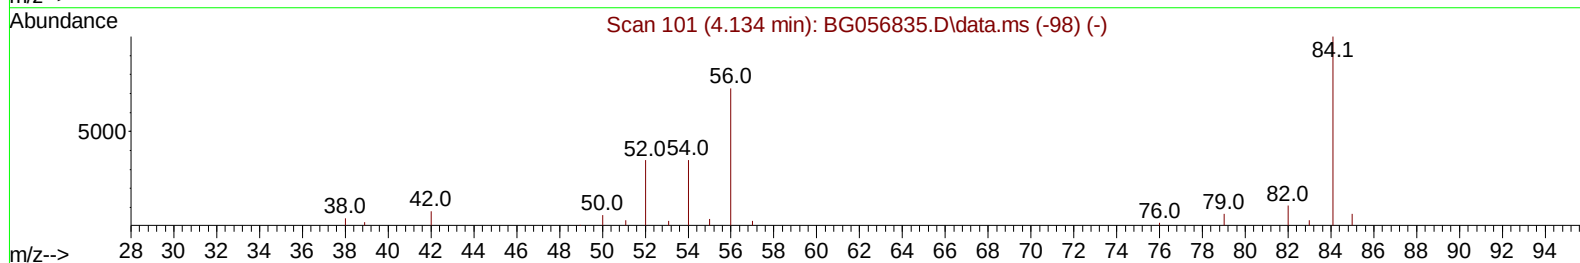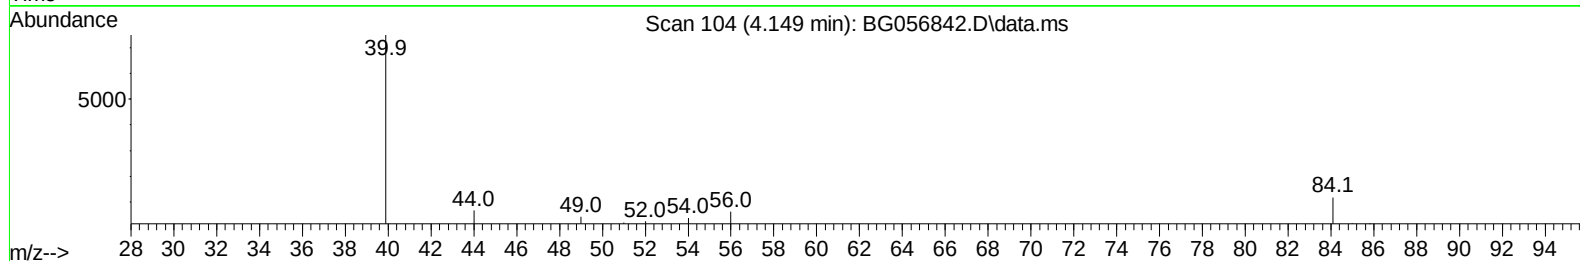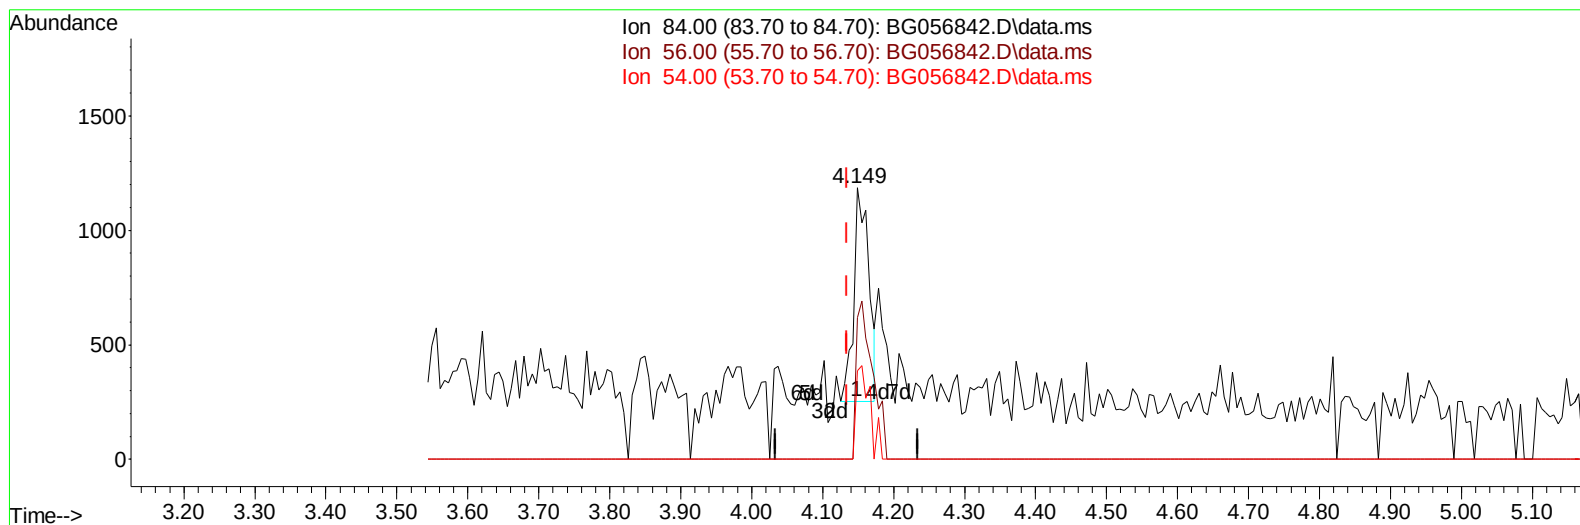

TIC: BG056842.D\data.ms

(4) Pyridine-d5 (S)

4.149min (+ 0.015) 1.09 ng/u1

response 1358

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	52.32#
54.00	38.20	32.57
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056842.D
Acq On : 6 Mar 2023 15:21
Operator : CG/JU
Sample : 01712-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX6

Manual IntegrationsAPPROVED

Quant Time: Mar 06 16:18:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

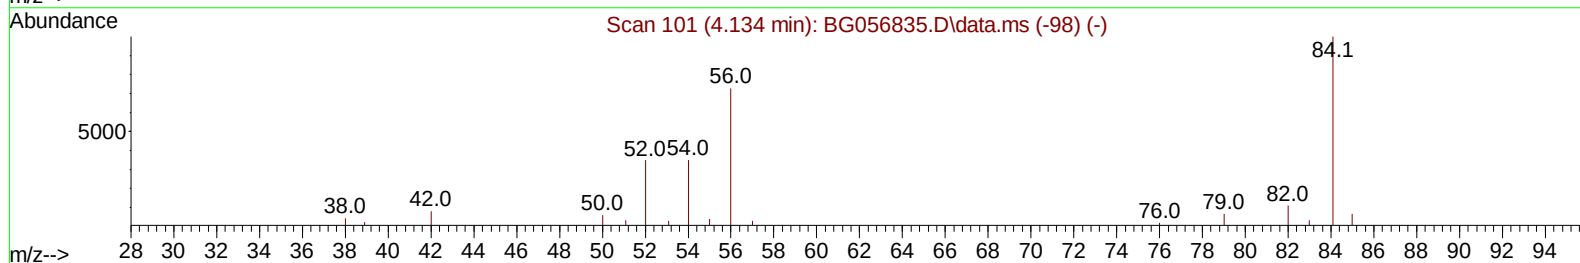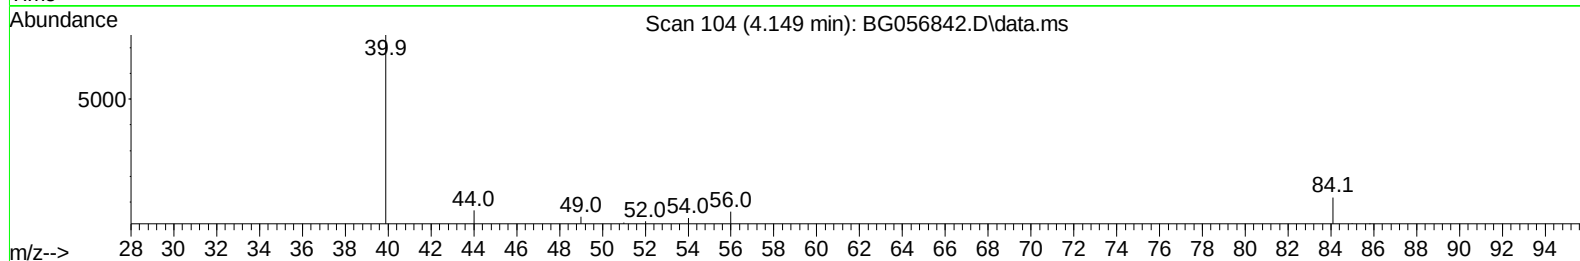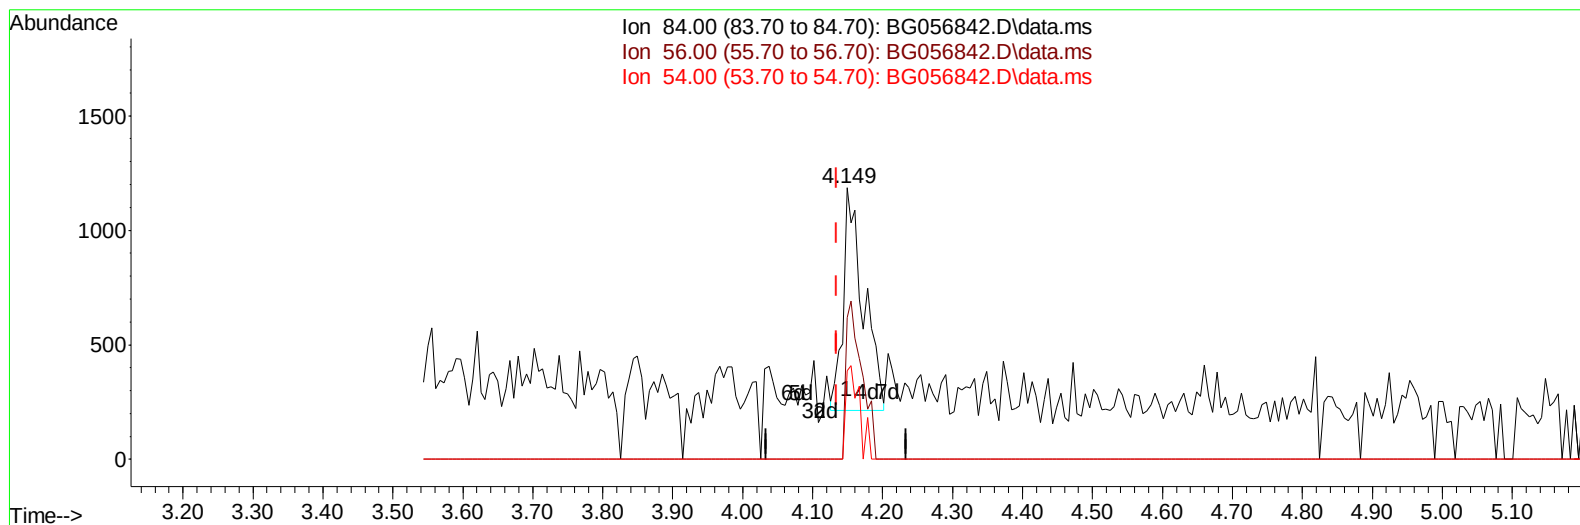

TIC: BG056842.D\data.ms

(4) Pyridine-d5 (S)

4.149min (+ 0.015) 1.56 ng/u1 m

response 1944

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	67.40	52.32#
54.00	38.20	32.57
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056842.D
 Acq On : 6 Mar 2023 15:21
 Operator : CG/JU
 Sample : 01712-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZX6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/07/2023
 Supervised By :Jagrut Upadhyay 03/07/2023

Quant Time: Mar 06 16:18:12 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.420	152	17076	20.000	ng/ul	0.00
20) Naphthalene-d8	11.258	136	75362	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.019	164	56940	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.757	188	124722	20.000	ng/ul	0.00
79) Chrysene-d12	22.063	240	105618	20.000	ng/ul	0.00
88) Perylene-d12	25.589	264	117770	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.697	96	789	2.563	ng/uL	0.00
4) Pyridine-d5	4.149	84	1944m	1.565	ng/ul	0.01
7) Phenol-d5	7.545	99	21677	12.686	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	14619	14.025	ng/ul	0.00
11) 2-Chlorophenol-d4	7.939	132	14768	13.014	ng/ul	0.00
15) 4-Methylphenol-d8	9.102	113	16953	12.984	ng/ul	0.00
21) Nitrobenzene-d5	9.590	128	9125	14.448	ng/ul	0.00
24) 2-Nitrophenol-d4	10.318	143	8125	10.808	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.865	165	18139	12.807	ng/ul	0.00
31) 4-Chloroaniline-d4	11.382	131	22207	12.022	ng/ul	0.00
46) Dimethylphthalate-d6	14.408	166	65411	14.238	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	78023	14.943	ng/ul	0.00
54) 4-Nitrophenol-d4	15.183	143	6163	7.781	ng/ul	0.00
60) Fluorene-d10	16.006	176	59241	13.940	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.105	200	4124	4.942	ng/ul	0.00
73) Anthracene-d10	17.851	188	94138	15.558	ng/ul	0.00
81) Pyrene-d10	20.113	212	109539	15.327	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.342	264	100666	15.836	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056842.D
Acq On : 6 Mar 2023 15:21
Operator : CG/JU
Sample : 01712-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX6

Manual IntegrationsAPPROVED

Quant Time: Mar 06 16:18:12 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

