




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056843.D
Acq On : 6 Mar 2023 16:02
Operator : CG/JU
Sample : 01712-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

Quant Time: Mar 06 16:53:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

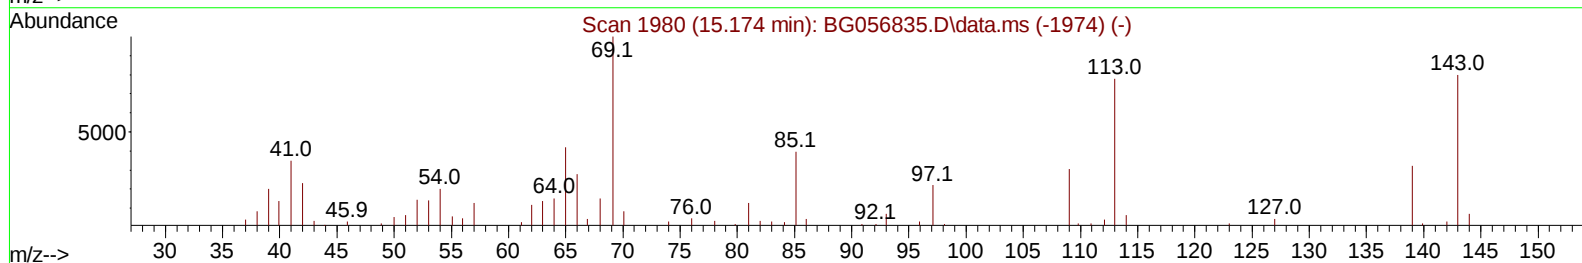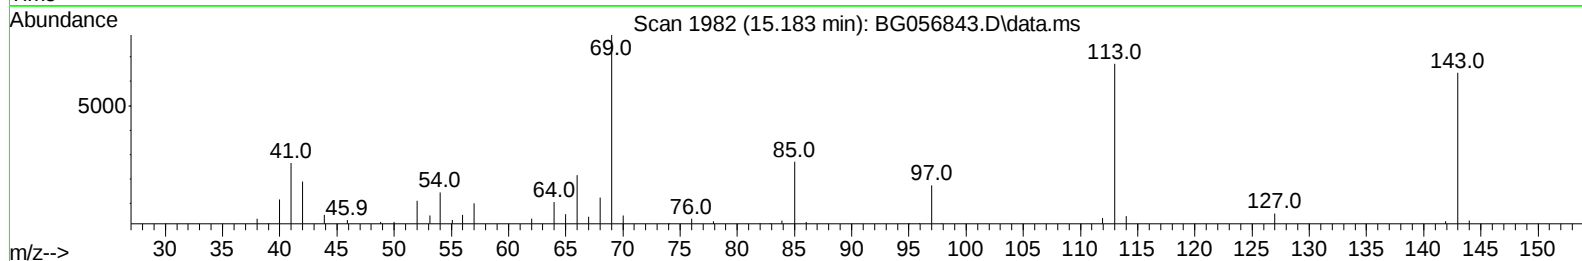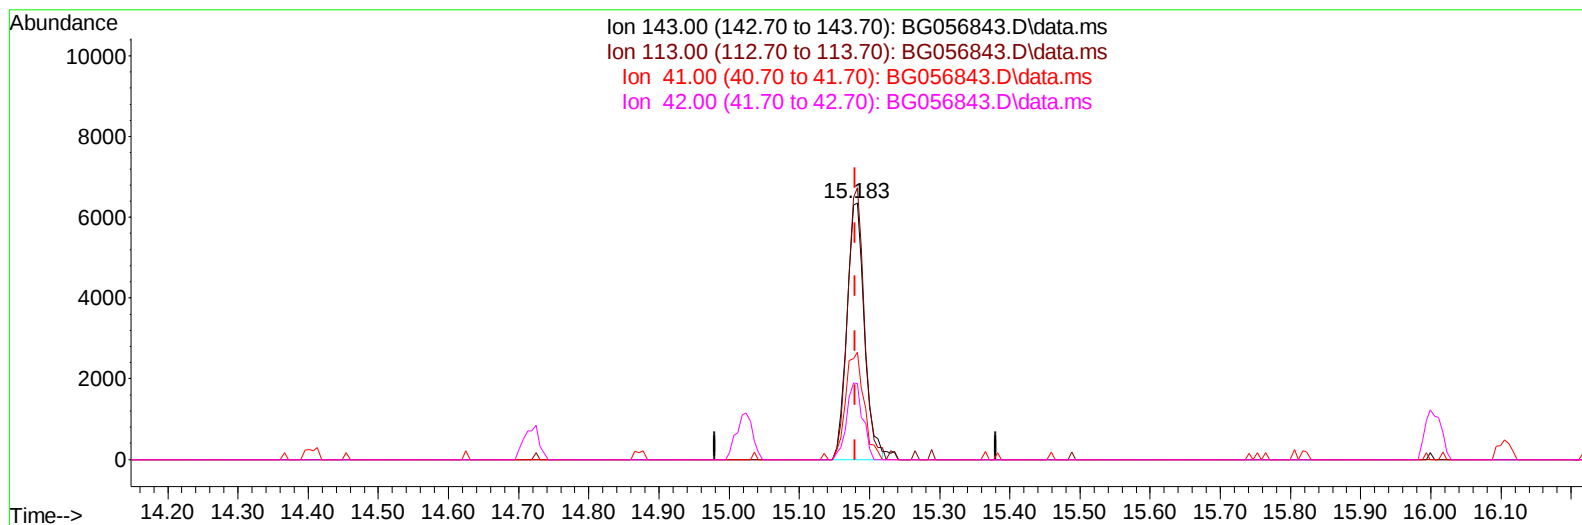

TIC: BG056843.D\data.ms

(54) 4-Nitrophenol-d4 (S)**15.183min (+ 0.003) 13.54 ng/u1****response 11041**

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.30	105.84
41.00	46.10	41.81
42.00	27.10	29.57




Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056843.D
Acq On : 6 Mar 2023 16:02
Operator : CG/JU
Sample : 01712-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

Quant Time: Mar 06 16:53:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

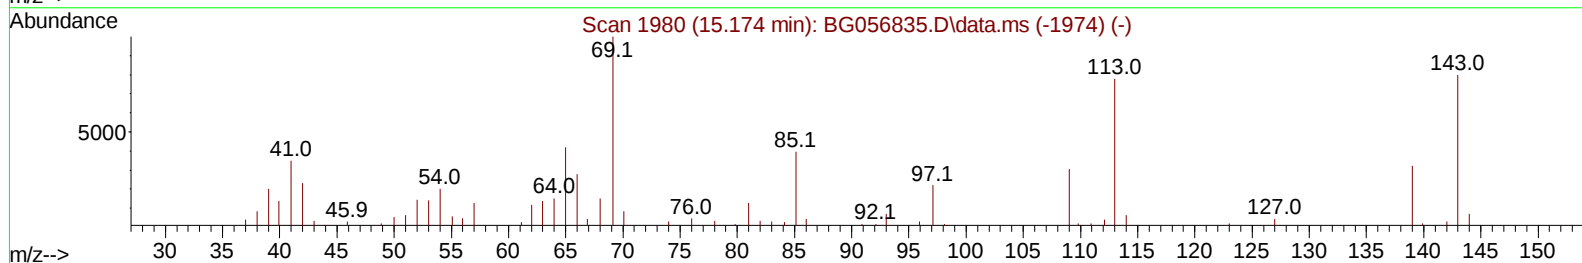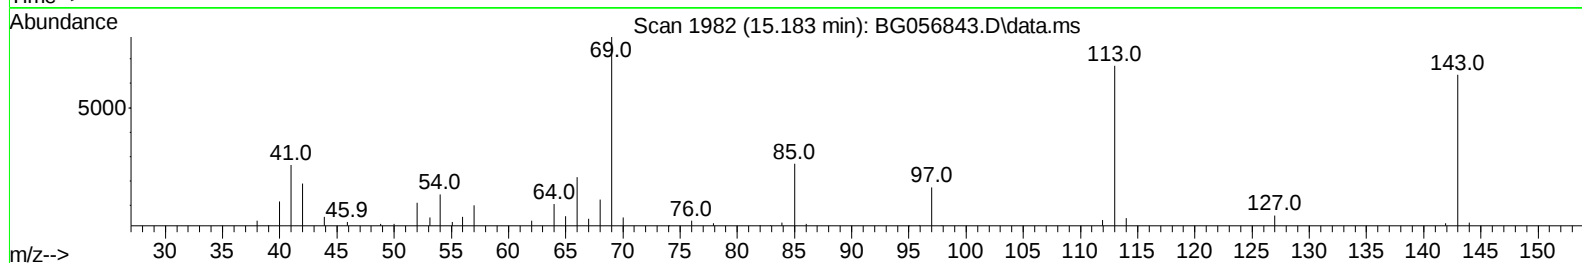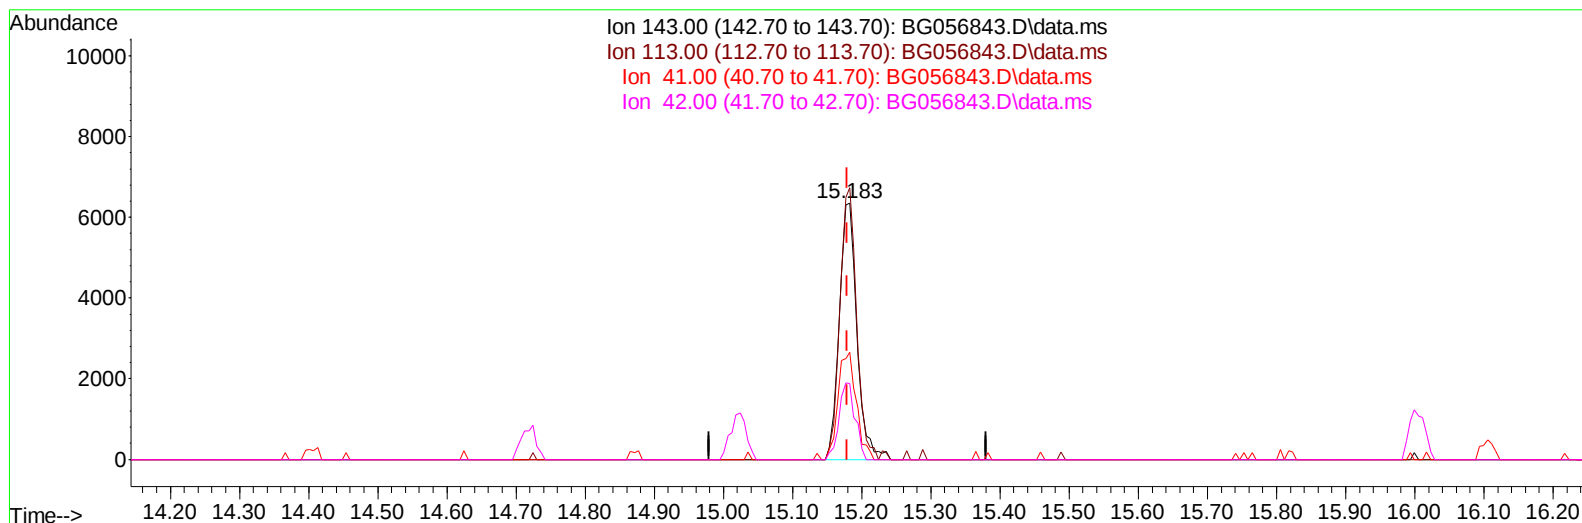

TIC: BG056843.D\data.ms

(54) 4-Nitrophenol-d4 (S)

15.183min (+ 0.003) 13.77 ng/ul m

response 11234

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	94.30	105.84
41.00	46.10	41.81
42.00	27.10	29.57

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056843.D
 Acq On : 6 Mar 2023 16:02
 Operator : CG/JU
 Sample : 01712-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DBZX7

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/07/2023
 Supervised By :Jagrut Upadhyay 03/07/2023

Quant Time: Mar 06 16:53:42 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 02 00:12:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.414	152	17034	20.000	ng/ul	0.00
20) Naphthalene-d8	11.252	136	81187	20.000	ng/ul	0.00
38) Acenaphthene-d10	15.024	164	58628	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.756	188	130597	20.000	ng/ul	0.00
79) Chrysene-d12	22.063	240	111709	20.000	ng/ul	0.00
88) Perylene-d12	25.588	264	121643	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.702	96	950	3.094	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.545	99	26188	15.363	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.721	67	16631	15.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.938	132	17918	15.829	ng/ul	0.00
15) 4-Methylphenol-d8	9.108	113	19140	14.695	ng/ul	0.00
21) Nitrobenzene-d5	9.589	128	10076	14.809	ng/ul	0.00
24) 2-Nitrophenol-d4	10.324	143	11873	14.660	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.858	165	22954	15.044	ng/ul	0.00
31) 4-Chloroaniline-d4	11.375	131	19566	9.832	ng/ul	0.00
46) Dimethylphthalate-d6	14.407	166	81074	17.139	ng/ul	0.00
49) Acenaphthylene-d8	14.719	160	89959	16.733	ng/ul	0.00
54) 4-Nitrophenol-d4	15.183	143	11234m	13.775	ng/ul	0.00
60) Fluorene-d10	16.005	176	72260	16.514	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	16.105	200	9477	10.846	ng/ul	0.00
73) Anthracene-d10	17.850	188	119892	18.923	ng/ul	0.00
81) Pyrene-d10	20.112	212	102611	13.574	ng/ul	0.00
92) Benzo(a)pyrene-d12	25.336	264	58149	8.856	ng/ul	-0.01

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056843.D
Acq On : 6 Mar 2023 16:02
Operator : CG/JU
Sample : 01712-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DBZX7

Manual IntegrationsAPPROVED

Quant Time: Mar 06 16:53:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 02 00:12:28 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/07/2023
Supervised By :Jagrut Upadhyay 03/07/2023

