

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056836.D
 Acq On : 6 Mar 2023 11:07
 Operator : CG/JU
 Sample : PB151218BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056836.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.134	98	101	113	rBV	57146	100049	19.87%	1.973%
2	6.232	457	458	460	rBV	1933	1329	0.26%	0.026%
3	7.536	674	680	690	rVB	66926	115460	22.93%	2.276%
4	7.718	705	711	720	rVB	50136	79333	15.76%	1.564%
5	7.936	742	748	759	rVB	58564	98876	19.64%	1.949%
6	8.218	794	796	797	rBV	994	707	0.14%	0.014%
7	8.412	823	829	837	rVB	56362	94194	18.71%	1.857%
8	9.105	940	947	956	rVB	79832	136223	27.06%	2.686%
9	9.587	1022	1029	1037	rVB	70781	121043	24.04%	2.386%
10	10.315	1147	1153	1160	rVB2	47125	80821	16.05%	1.593%
11	10.856	1238	1245	1254	rBV	82308	141980	28.20%	2.799%
12	11.249	1304	1312	1321	rVB	81052	148273	29.45%	2.923%
13	11.373	1326	1333	1342	rVB	86841	153507	30.49%	3.027%
14	12.801	1573	1576	1580	rVB2	1159	1798	0.36%	0.035%
15	14.187	1808	1812	1814	rVB2	540	777	0.15%	0.015%
16	14.405	1843	1849	1855	rBV	173346	245244	48.71%	4.835%
17	14.716	1895	1902	1909	rBV	195364	302250	60.04%	5.959%
18	15.016	1946	1953	1960	rBV	160781	244177	48.50%	4.814%
19	15.174	1973	1980	1990	rBV	68083	109576	21.76%	2.160%
20	15.797	2082	2086	2090	rBV2	419	773	0.15%	0.015%
21	15.997	2114	2120	2127	rVB	244937	377955	75.07%	7.452%
22	16.097	2132	2137	2147	rVB2	53418	79877	15.87%	1.575%
23	16.238	2157	2161	2163	rBV2	724	684	0.14%	0.013%
24	16.532	2207	2211	2214	rBV	416	686	0.14%	0.014%
25	17.272	2332	2337	2340	rVB	482	712	0.14%	0.014%
26	17.748	2412	2418	2427	rVB	203381	316539	62.87%	6.241%
27	17.848	2427	2435	2442	rBV2	283403	425115	84.44%	8.382%
28	17.983	2456	2458	2461	rVB	633	696	0.14%	0.014%
29	18.171	2487	2490	2492	rBV	682	697	0.14%	0.014%
30	18.517	2546	2549	2551	rBV	618	699	0.14%	0.014%
31	18.594	2560	2562	2567	rBV2	469	779	0.15%	0.015%
32	18.776	2591	2593	2596	rVB	900	823	0.16%	0.016%
33	18.811	2596	2599	2600	rBV	776	712	0.14%	0.014%
34	19.675	2741	2746	2751	rBV4	3154	4574	0.91%	0.090%
35	19.745	2754	2758	2762	rVB4	3905	4731	0.94%	0.093%
36	19.822	2768	2771	2774	rBV3	738	1335	0.27%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056836.D
 Acq On : 6 Mar 2023 11:07
 Operator : CG/JU
 Sample : PB151218BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	19.975	2795	2797	2798	rBV	737	697	0.14%	0.014%
38	20.110	2813	2820	2826	rBV	353116	503454	100.00%	9.926%
39	20.233	2840	2841	2843	rBV2	1333	720	0.14%	0.014%
40	20.351	2859	2861	2864	rBV3	969	845	0.17%	0.017%
41	20.427	2872	2874	2877	rBV4	1106	948	0.19%	0.019%
42	20.492	2884	2885	2887	rBV2	1229	825	0.16%	0.016%
43	20.527	2889	2891	2894	rVB2	1239	999	0.20%	0.020%
44	20.915	2956	2957	2959	rBV2	1264	1057	0.21%	0.021%
45	21.279	3017	3019	3020	rBV	1414	749	0.15%	0.015%
46	22.054	3144	3151	3158	rBV2	201934	340566	67.65%	6.715%
47	24.646	3590	3592	3593	rBV2	2008	935	0.19%	0.018%
48	25.333	3697	3709	3721	rBV2	160188	475501	94.45%	9.375%
49	25.574	3740	3750	3765	rVB2	110402	338815	67.30%	6.680%
50	25.921	3807	3809	3810	rBV2	1836	835	0.17%	0.016%
51	25.997	3820	3822	3825	rBV2	1665	1632	0.32%	0.032%
52	27.237	4031	4033	4037	rBV4	1660	2001	0.40%	0.039%
53	27.619	4096	4098	4099	rBV2	1663	771	0.15%	0.015%
54	28.876	4310	4312	4314	rBV3	1744	1426	0.28%	0.028%
55	29.117	4351	4353	4354	rBV	1619	859	0.17%	0.017%
56	29.945	4492	4494	4495	rBV2	2484	1564	0.31%	0.031%
57	30.092	4517	4519	4520	rBV	1914	921	0.18%	0.018%
58	31.250	4714	4716	4719	rVB2	2903	2875	0.57%	0.057%




Sum of corrected areas: 5071999

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056836.D
Acq On : 6 Mar 2023 11:07
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

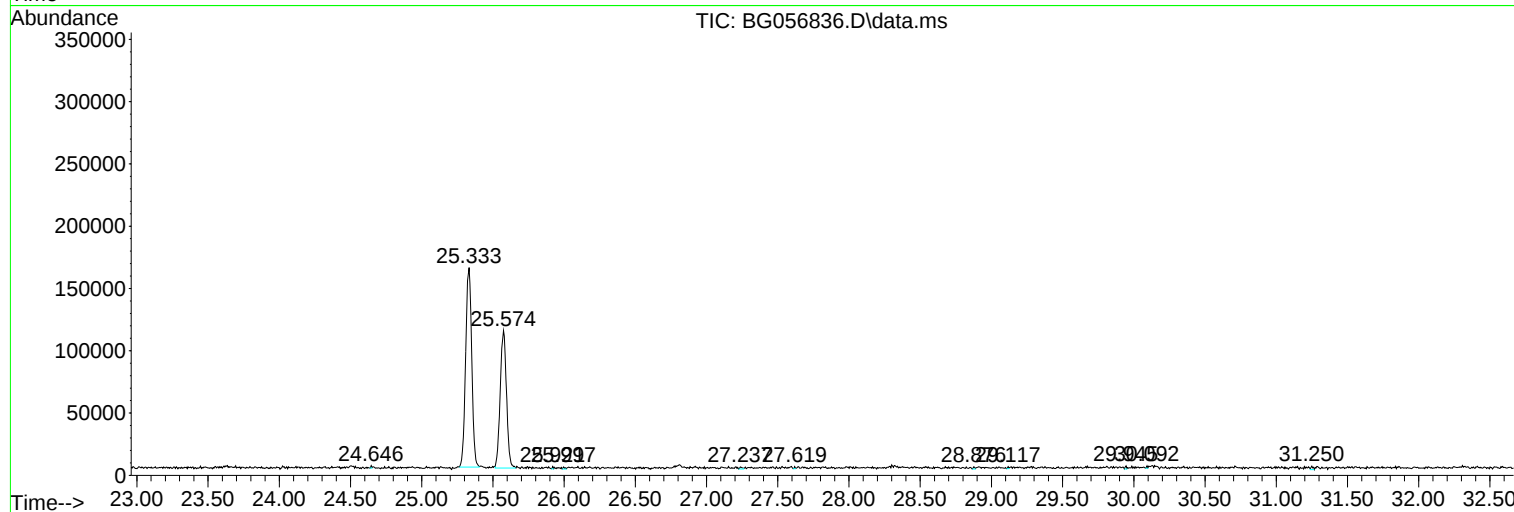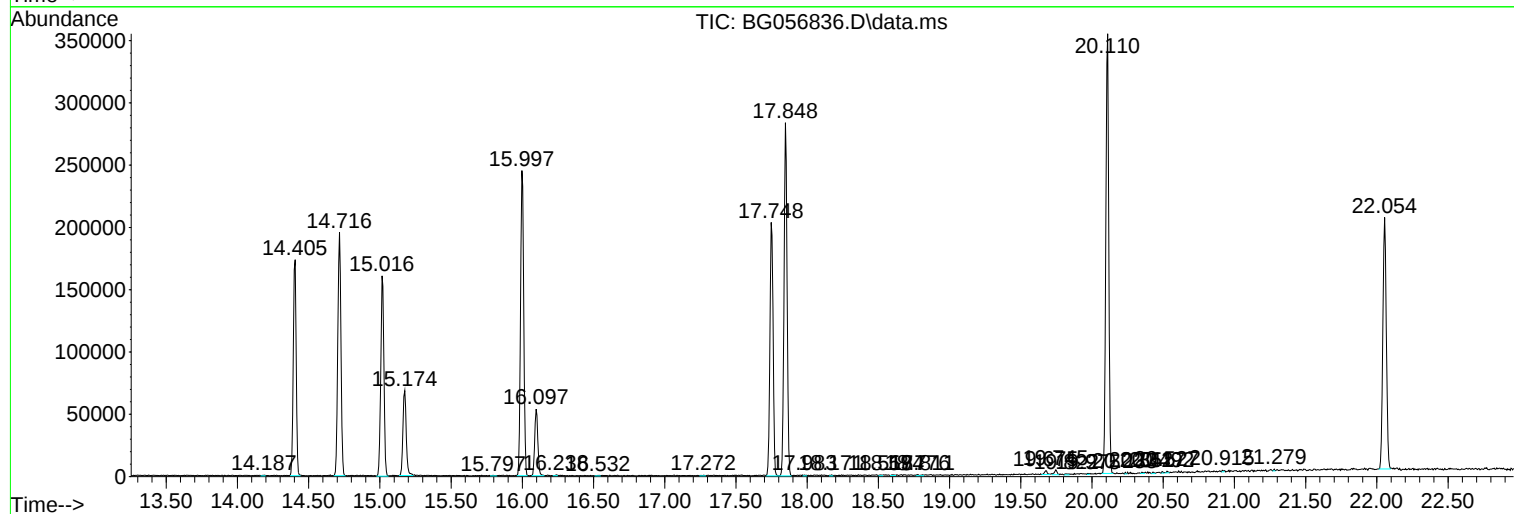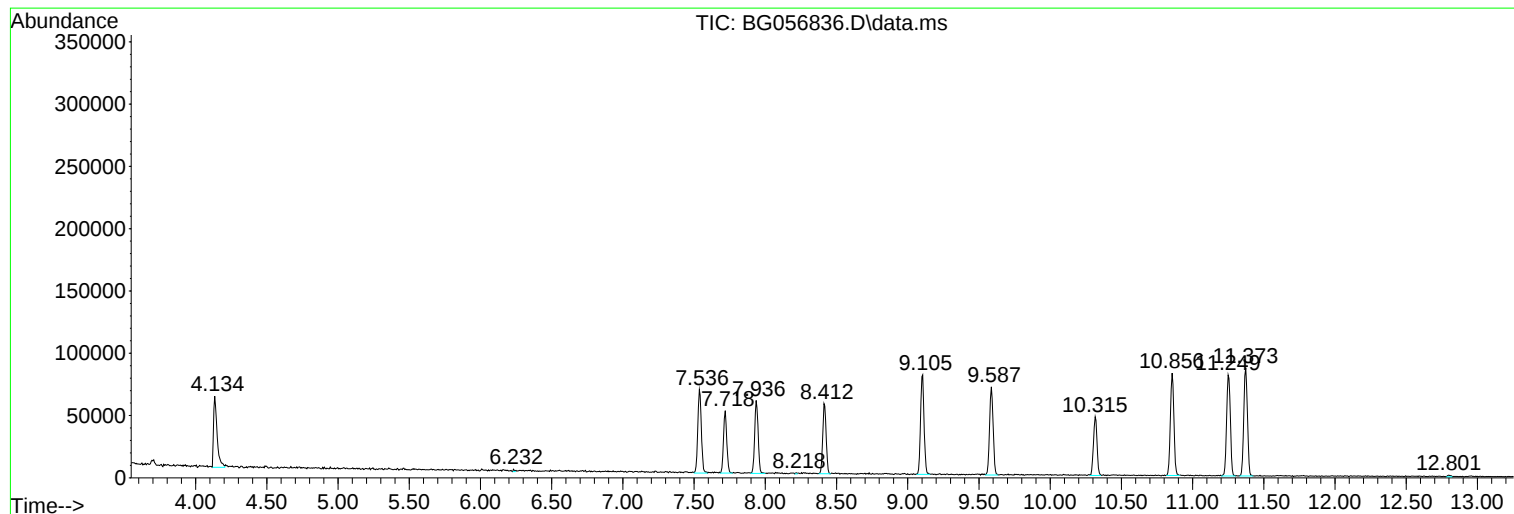

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056836.D
Acq On : 6 Mar 2023 11:07
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056836.D
Acq On : 6 Mar 2023 11:07
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc