

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056846.D
 Acq On : 6 Mar 2023 18:06
 Operator : CG/JU
 Sample : PB151218BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056846.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.139	98	102	115	rVB	59207	100301	20.03%	1.792%
2	7.541	675	681	688	rVB	89082	152501	30.45%	2.725%
3	7.718	706	711	718	rVB	56974	97428	19.45%	1.741%
4	7.941	742	749	756	rBV	79981	137247	27.40%	2.452%
5	8.417	825	830	838	rVB	73736	122346	24.43%	2.186%
6	8.476	838	840	843	rBV	1218	1182	0.24%	0.021%
7	9.104	941	947	955	rVB	105896	183985	36.73%	3.287%
8	9.592	1023	1030	1040	rVB	88214	154847	30.92%	2.767%
9	9.839	1070	1072	1077	rBV2	793	1073	0.21%	0.019%
10	9.939	1087	1089	1091	rBV2	919	857	0.17%	0.015%
11	10.320	1148	1154	1161	rBV2	71936	130795	26.11%	2.337%
12	10.861	1239	1246	1258	rVB	115532	197682	39.47%	3.532%
13	11.255	1306	1313	1322	rVB	102906	182628	36.46%	3.263%
14	11.378	1327	1334	1342	rVB	104376	190343	38.00%	3.401%
15	11.590	1366	1370	1371	rBV3	704	786	0.16%	0.014%
16	11.754	1395	1398	1400	rVB	855	680	0.14%	0.012%
17	11.889	1417	1421	1423	rBV	471	706	0.14%	0.013%
18	12.342	1494	1498	1501	rVB3	599	705	0.14%	0.013%
19	12.453	1514	1517	1520	rBV2	612	749	0.15%	0.013%
20	12.806	1574	1577	1578	rBV2	1159	1322	0.26%	0.024%
21	14.404	1843	1849	1857	rBV	195120	285881	57.08%	5.108%
22	14.721	1892	1903	1911	rBV	217659	344936	68.87%	6.163%
23	15.021	1948	1954	1961	rVB	174783	268449	53.60%	4.796%
24	15.179	1975	1981	1992	rBV	82561	134033	26.76%	2.395%
25	15.356	2008	2011	2014	rBV2	613	908	0.18%	0.016%
26	15.473	2027	2031	2034	rBV2	541	720	0.14%	0.013%
27	16.002	2115	2121	2128	rVB	278237	414744	82.81%	7.410%
28	16.102	2133	2138	2144	rBV	59751	89447	17.86%	1.598%
29	16.261	2162	2165	2167	rVB	591	688	0.14%	0.012%
30	16.642	2227	2230	2233	rBV2	714	865	0.17%	0.015%
31	17.547	2383	2384	2387	rVB	935	804	0.16%	0.014%
32	17.606	2390	2394	2397	rVB	716	1062	0.21%	0.019%
33	17.753	2412	2419	2425	rBV	209883	318449	63.58%	5.690%
34	17.853	2430	2436	2446	rVB	296908	436600	87.17%	7.801%
35	18.229	2497	2500	2503	rVB	783	899	0.18%	0.016%
36	18.299	2507	2512	2515	rBV	546	1074	0.21%	0.019%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056846.D
 Acq On : 6 Mar 2023 18:06
 Operator : CG/JU
 Sample : PB151218BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK218

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	18.511	2544	2548	2549	rBV2	743	772	0.15%	0.014%
38	18.623	2563	2567	2569	rBV2	785	743	0.15%	0.013%
39	18.805	2595	2598	2601	rBV2	1529	1483	0.30%	0.026%
40	18.875	2605	2610	2614	rBV2	1284	1621	0.32%	0.029%
41	18.946	2618	2622	2624	rBV	987	1420	0.28%	0.025%
42	19.034	2635	2637	2642	rVB	920	978	0.20%	0.017%
43	19.151	2656	2657	2660	rBV	811	838	0.17%	0.015%
44	19.210	2666	2667	2670	rVB2	1146	900	0.18%	0.016%
45	19.251	2673	2674	2677	rVB2	1071	854	0.17%	0.015%
46	19.292	2679	2681	2684	rVV2	839	924	0.18%	0.017%
47	19.328	2686	2687	2692	rVB2	924	1084	0.22%	0.019%
48	19.369	2692	2694	2696	rBV2	955	823	0.16%	0.015%
49	19.386	2696	2697	2700	rBV	790	858	0.17%	0.015%
50	19.504	2715	2717	2719	rBV	1239	1495	0.30%	0.027%
51	19.574	2727	2729	2731	rBV	924	816	0.16%	0.015%
52	19.615	2735	2736	2739	rBV3	1497	1577	0.31%	0.028%
53	19.680	2743	2747	2753	rVB5	3850	7168	1.43%	0.128%
54	19.751	2753	2759	2765	rBV3	4364	8730	1.74%	0.156%
55	19.821	2769	2771	2772	rBV2	1679	1268	0.25%	0.023%
56	19.903	2783	2785	2787	rVB3	1928	1181	0.24%	0.021%
57	19.921	2787	2788	2790	rBV2	1951	1296	0.26%	0.023%
58	20.115	2814	2821	2829	rBV	349666	500862	100.00%	8.949%
59	20.215	2836	2838	2840	rBV3	1297	941	0.19%	0.017%
60	20.362	2860	2863	2864	rBV2	2162	2280	0.46%	0.041%
61	20.873	2948	2950	2953	rVB3	2734	2322	0.46%	0.041%
62	22.066	3146	3153	3160	rVB2	180620	319153	63.72%	5.702%
63	25.344	3702	3711	3724	rVB2	158540	455265	90.90%	8.134%
64	25.585	3743	3752	3765	rVB2	102249	321656	64.22%	5.747%




Sum of corrected areas: 5597030

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056846.D
Acq On : 6 Mar 2023 18:06
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

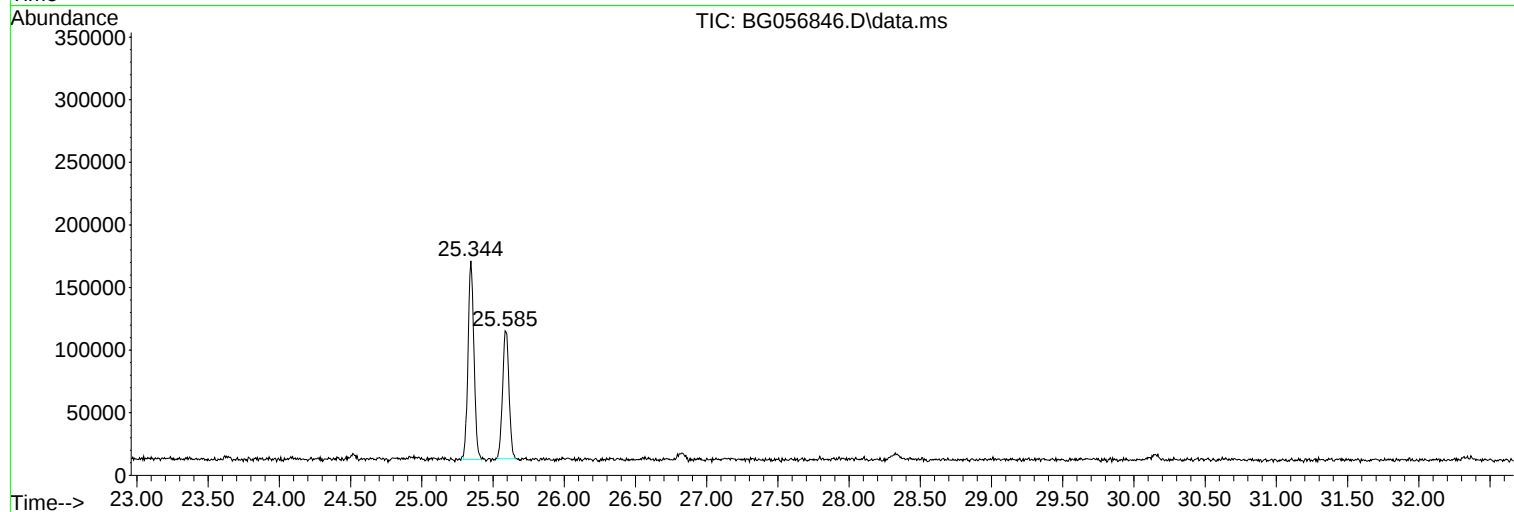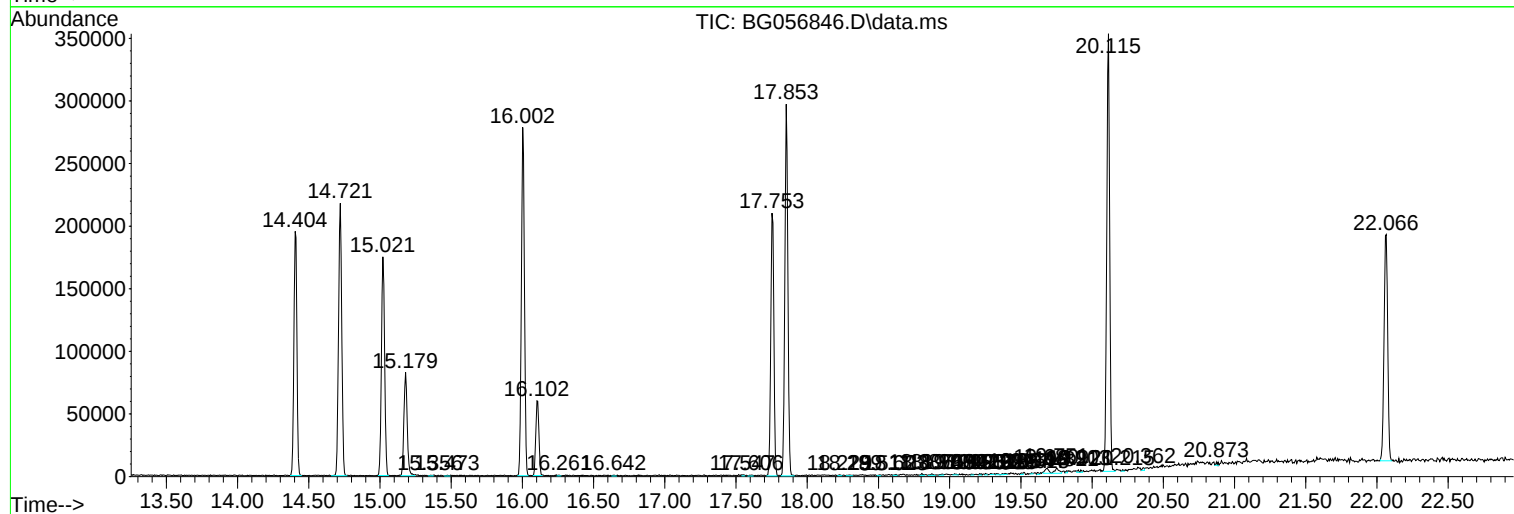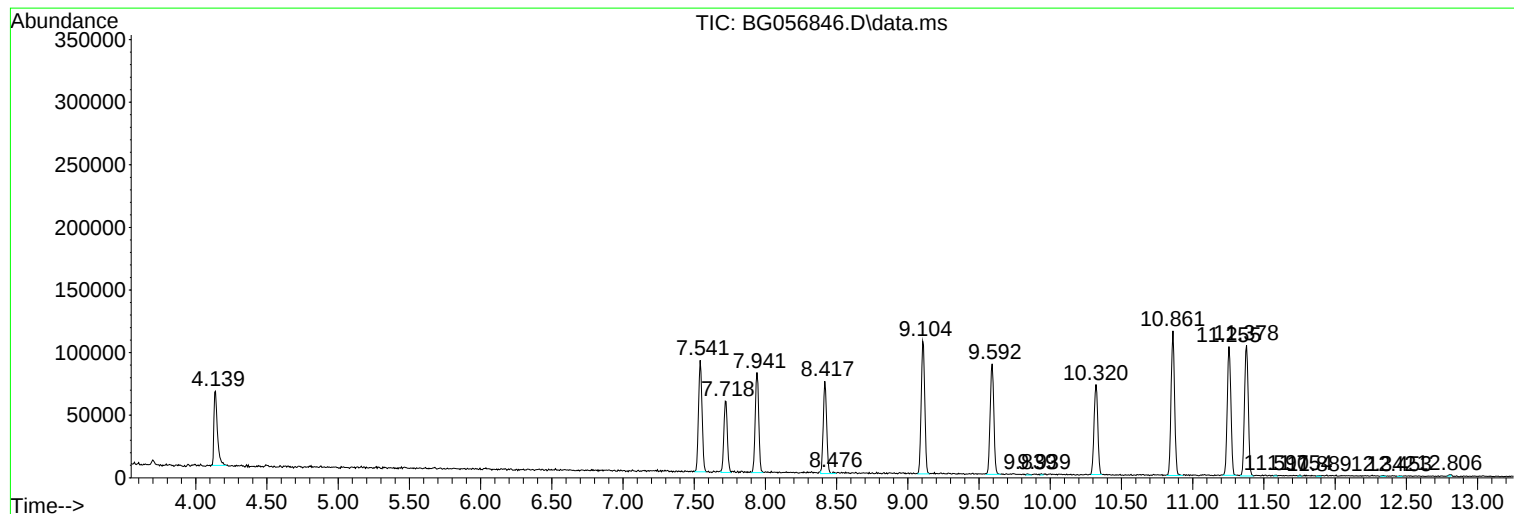

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056846.D
Acq On : 6 Mar 2023 18:06
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056846.D
Acq On : 6 Mar 2023 18:06
Operator : CG/JU
Sample : PB151218BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK218

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc