

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056862.D
 Acq On : 7 Mar 2023 5:48
 Operator : CG/JU
 Sample : PB151158BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

Signal : TIC: BG056862.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.611	8	12	19	rVB	101915	122931	36.82%	7.362%
2	8.411	824	829	835	rVB	62092	102672	30.75%	6.149%
3	8.805	894	896	897	rVB	1245	675	0.20%	0.040%
4	9.116	947	949	952	rBV	805	1085	0.33%	0.065%
5	9.363	989	991	993	rBV	836	635	0.19%	0.038%
6	9.480	1009	1011	1013	rBV	773	497	0.15%	0.030%
7	10.080	1111	1113	1117	rBV	766	720	0.22%	0.043%
8	10.661	1210	1212	1214	rBV2	579	469	0.14%	0.028%
9	11.073	1280	1282	1287	rVB2	585	1064	0.32%	0.064%
10	11.114	1287	1289	1291	rBV	634	603	0.18%	0.036%
11	11.255	1306	1313	1320	rVB	90899	154390	46.25%	9.246%
12	11.689	1384	1387	1388	rBV	558	626	0.19%	0.037%
13	11.848	1412	1414	1418	rBV2	576	864	0.26%	0.052%
14	11.889	1418	1421	1422	rVV2	557	515	0.15%	0.031%
15	12.923	1594	1597	1601	rVB2	508	698	0.21%	0.042%
16	13.276	1656	1657	1660	rBV2	453	503	0.15%	0.030%
17	13.481	1687	1692	1695	rBV2	500	765	0.23%	0.046%
18	13.552	1701	1704	1707	rVB2	369	433	0.13%	0.026%
19	13.711	1729	1731	1735	rBV2	377	440	0.13%	0.026%
20	13.863	1755	1757	1761	rBV2	379	513	0.15%	0.031%
21	14.028	1782	1785	1787	rBV	528	569	0.17%	0.034%
22	14.145	1803	1805	1806	rBV	541	435	0.13%	0.026%
23	14.251	1819	1823	1825	rBV2	390	496	0.15%	0.030%
24	14.380	1843	1845	1848	rVB2	357	468	0.14%	0.028%
25	14.486	1860	1863	1865	rBV2	316	433	0.13%	0.026%
26	14.927	1936	1938	1941	rVB2	453	500	0.15%	0.030%
27	15.021	1947	1954	1961	rBV	155775	240172	71.94%	14.384%
28	15.603	2048	2053	2054	rBV2	415	620	0.19%	0.037%
29	15.932	2105	2109	2110	rBV2	631	813	0.24%	0.049%
30	16.167	2148	2149	2153	rVB	541	511	0.15%	0.031%
31	16.219	2153	2158	2159	rVB	491	523	0.16%	0.031%
32	16.243	2159	2162	2163	rBV	495	434	0.13%	0.026%
33	16.266	2163	2166	2169	rVB2	500	622	0.19%	0.037%
34	16.507	2204	2207	2208	rBV2	470	467	0.14%	0.028%
35	16.607	2221	2224	2225	rBV	615	473	0.14%	0.028%
36	16.654	2231	2232	2235	rBV2	467	433	0.13%	0.026%

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056862.D
 Acq On : 7 Mar 2023 5:48
 Operator : CG/JU
 Sample : PB151158BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

37	16.748	2246	2248	2254	rVB	367	523	0.16%	0.031%
38	16.925	2275	2278	2279	rBV	373	443	0.13%	0.027%
39	17.077	2302	2304	2307	rVB	544	632	0.19%	0.038%
40	17.101	2307	2308	2311	rBV	481	466	0.14%	0.028%

41	17.171	2319	2320	2323	rVB	638	517	0.15%	0.031%
42	17.195	2323	2324	2327	rBV	533	588	0.18%	0.035%
43	17.418	2360	2362	2365	rVB	629	768	0.23%	0.046%
44	17.447	2365	2367	2369	rBV	673	708	0.21%	0.042%
45	17.465	2369	2370	2373	rVB	598	450	0.13%	0.027%

46	17.500	2373	2376	2378	rBV	519	744	0.22%	0.045%
47	17.583	2386	2390	2392	rBV2	623	890	0.27%	0.053%
48	17.694	2405	2409	2413	rBV	402	542	0.16%	0.032%
49	17.753	2413	2419	2426	rVV	213310	315239	94.43%	18.880%
50	17.912	2444	2446	2448	rBV	637	597	0.18%	0.036%

51	17.970	2453	2456	2459	rBV2	577	684	0.20%	0.041%
52	18.058	2467	2471	2472	rBV	636	557	0.17%	0.033%
53	18.129	2481	2483	2485	rBV	723	602	0.18%	0.036%
54	18.205	2495	2496	2499	rBV2	510	482	0.14%	0.029%
55	18.329	2516	2517	2520	rBV	510	548	0.16%	0.033%

56	18.364	2521	2523	2525	rVB2	607	538	0.16%	0.032%
57	18.387	2525	2527	2529	rBV	679	537	0.16%	0.032%
58	18.482	2542	2543	2546	rBV2	764	841	0.25%	0.050%
59	18.564	2555	2557	2559	rVB	782	576	0.17%	0.034%
60	18.652	2569	2572	2575	rBV	604	834	0.25%	0.050%

61	18.711	2580	2582	2584	rVB	739	595	0.18%	0.036%
62	18.781	2592	2594	2596	rVB	639	504	0.15%	0.030%
63	18.834	2598	2603	2604	rBV2	809	795	0.24%	0.048%
64	18.858	2604	2607	2610	rBV	682	635	0.19%	0.038%
65	19.151	2653	2657	2660	rVB2	723	876	0.26%	0.052%

66	19.222	2664	2669	2671	rBV2	488	881	0.26%	0.053%
67	19.316	2681	2685	2686	rBV	466	562	0.17%	0.034%
68	19.386	2695	2697	2700	rVB	662	638	0.19%	0.038%
69	19.445	2705	2707	2710	rVB2	728	814	0.24%	0.049%
70	19.480	2710	2713	2715	rBV2	685	871	0.26%	0.052%

71	19.527	2718	2721	2723	rBV2	582	458	0.14%	0.027%
72	19.662	2741	2744	2745	rVB	746	663	0.20%	0.040%
73	19.721	2752	2754	2758	rVB2	534	661	0.20%	0.040%
74	19.839	2772	2774	2775	rVB2	756	529	0.16%	0.032%
75	19.903	2784	2785	2788	rVB2	845	715	0.21%	0.043%

76	19.950	2791	2793	2796	rVV2	702	845	0.25%	0.051%
----	--------	------	------	------	------	-----	-----	-------	--------

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
 Data File : BG056862.D
 Acq On : 7 Mar 2023 5:48
 Operator : CG/JU
 Sample : PB151158BL
 Misc : GCMS CONFIRMATION
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK158

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
 Title : SVOA CALIBRATION

77	20.062	2809	2812	2815	rBV2	1429	1812	0.54%	0.109%
78	20.150	2824	2827	2828	rVB2	761	755	0.23%	0.045%
79	20.285	2848	2850	2852	rVB2	878	672	0.20%	0.040%
80	20.426	2873	2874	2876	rBV	1152	905	0.27%	0.054%
81	20.497	2883	2886	2887	rBV2	1205	1163	0.35%	0.070%
82	20.520	2887	2890	2891	rBV2	1298	1167	0.35%	0.070%
83	20.767	2930	2932	2934	rVB	1685	1352	0.40%	0.081%
84	20.791	2934	2936	2938	rBV2	1550	1517	0.45%	0.091%
85	20.814	2938	2940	2941	rBV	1569	1126	0.34%	0.067%
86	20.908	2955	2956	2957	rBV	1466	628	0.19%	0.038%
87	21.131	2993	2994	2996	rBV2	2616	1786	0.53%	0.107%
88	22.060	3146	3152	3162	rVB2	190852	333845	100.00%	19.994%
89	22.160	3167	3169	3171	rBV3	2312	1494	0.45%	0.089%
90	23.558	3405	3407	3408	rBV2	2148	1214	0.36%	0.073%
91	24.163	3508	3510	3511	rBV2	1876	1596	0.48%	0.096%
92	24.245	3523	3524	3526	rBV2	2460	2196	0.66%	0.132%
93	25.591	3742	3753	3765	rVB2	104490	325956	97.64%	19.522%
94	25.890	3802	3804	3806	rBV3	1952	1640	0.49%	0.098%
95	26.419	3892	3894	3897	rBV3	2386	1908	0.57%	0.114%
96	27.101	4008	4010	4012	rBV2	1831	1286	0.39%	0.077%
97	28.975	4327	4329	4330	rBV	1818	1469	0.44%	0.088%
98	29.140	4355	4357	4360	rBV4	1800	1331	0.40%	0.080%
99	30.138	4525	4527	4529	rBV2	2412	2242	0.67%	0.134%
100	31.178	4702	4704	4705	rBV2	1645	1245	0.37%	0.075%




Sum of corrected areas: 1669720

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056862.D
Acq On : 7 Mar 2023 5:48
Operator : CG/JU
Sample : PB151158BL
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

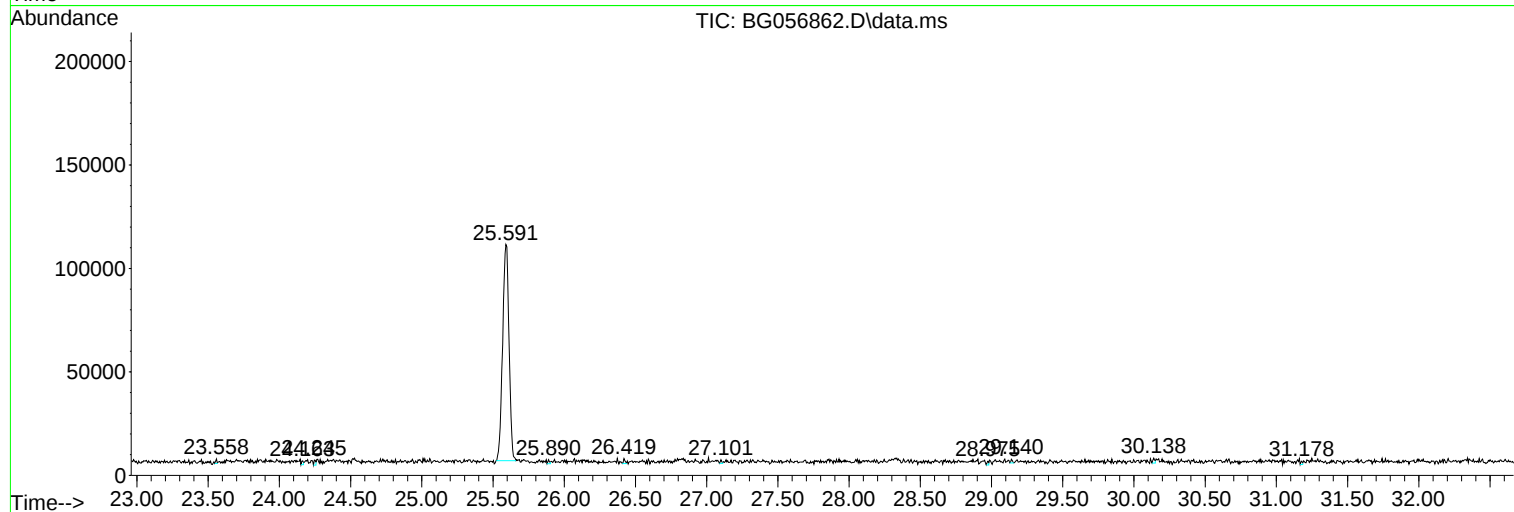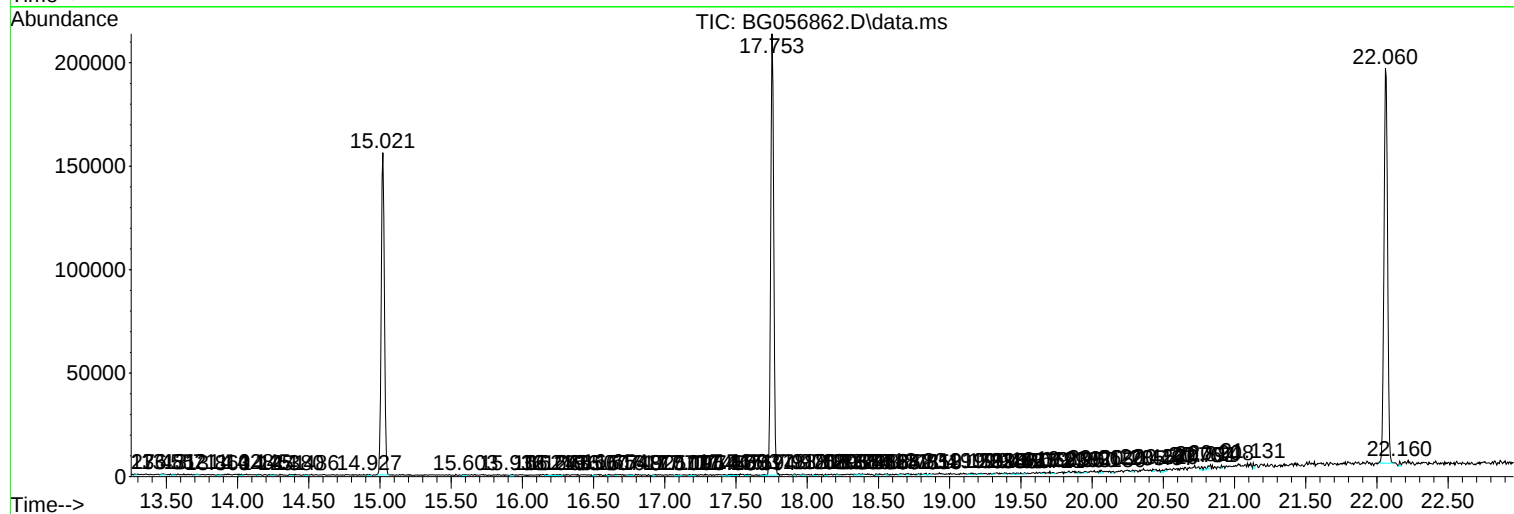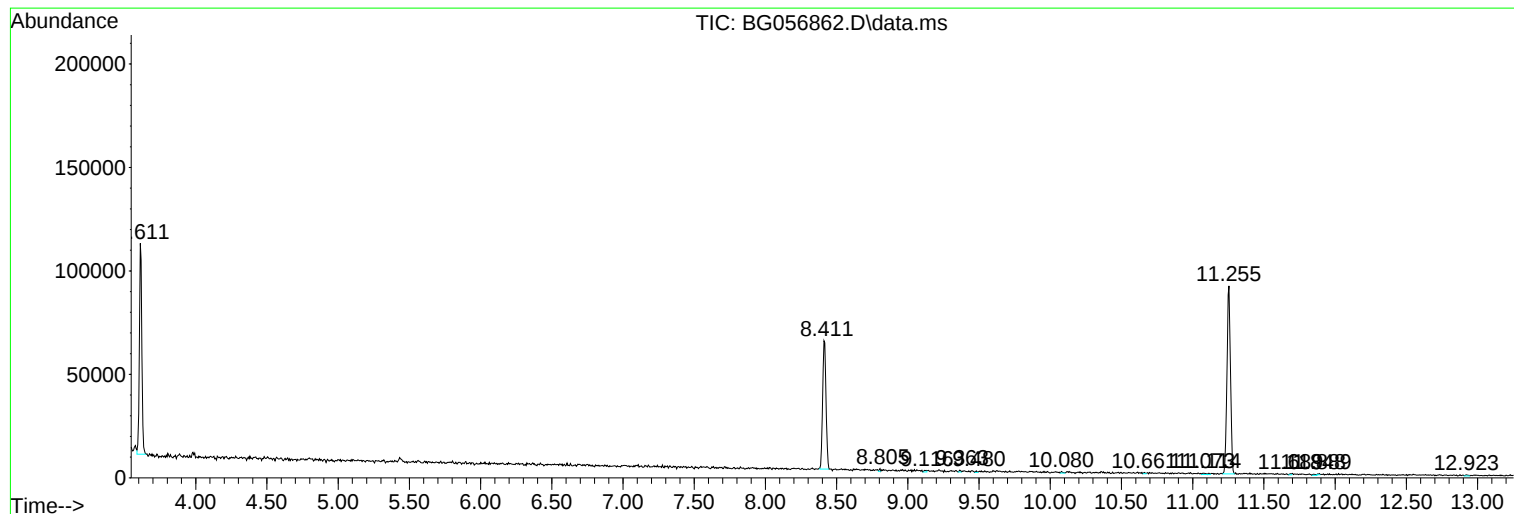

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056862.D
Acq On : 7 Mar 2023 5:48
Operator : CG/JU
Sample : PB151158BL
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK158










Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.611	23.95 ng/ul	122931	1,4-Dichlorobenzene-d4	8.417

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	91
2	Heptane			100	C7H16	000142-82-5	87
3	Heptane			100	C7H16	000142-82-5	87
4	Heptane			100	C7H16	000142-82-5	72
5	Heptane, 2,4-dimethyl-			128	C9H20	002213-23-2	64

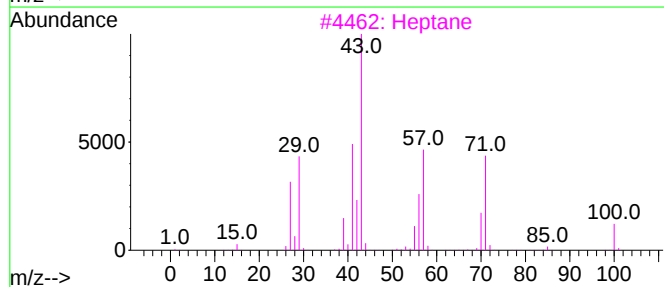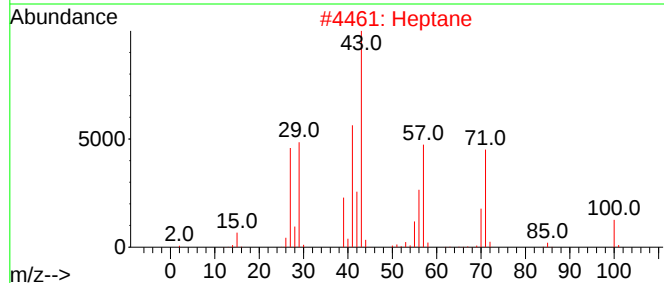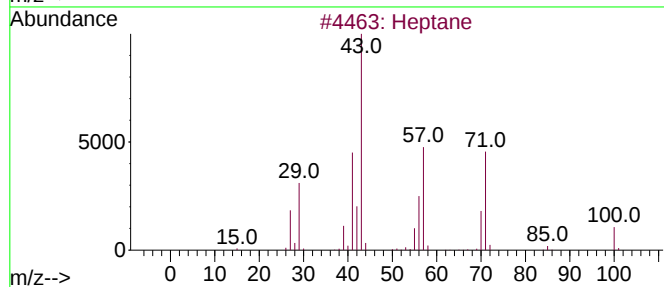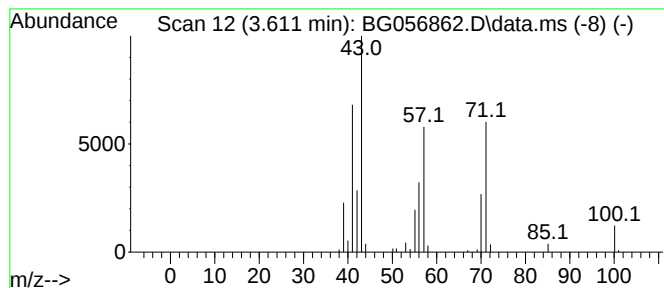

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030623\
Data File : BG056862.D
Acq On : 7 Mar 2023 5:48
Operator : CG/JU
Sample : PB151158BL
Misc : GCMS CONFIRMATION
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK158

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\SFAM-EPA-BG022323.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.611	23.9	ng/u1	122931	1	8.417	102672	20.0