
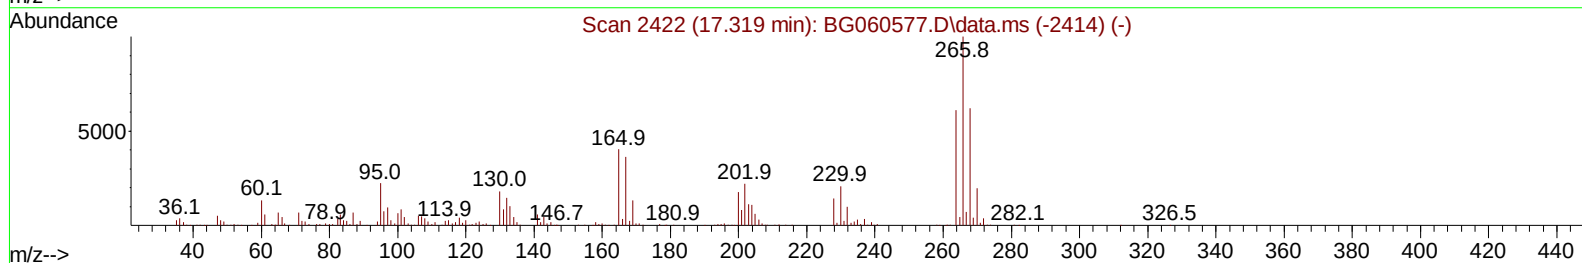
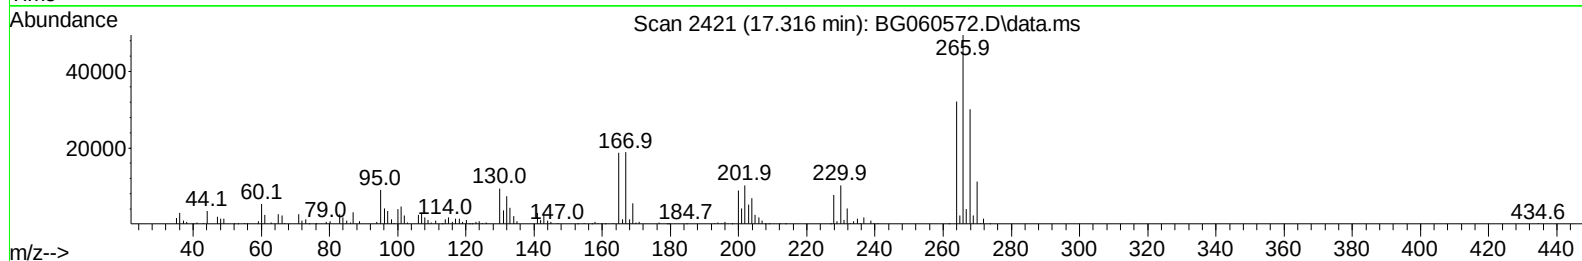


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030624\
Data File : BG060572.D
Acq On : 6 Mar 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:05:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 02:50:02 2024
Response via : Initial Calibration

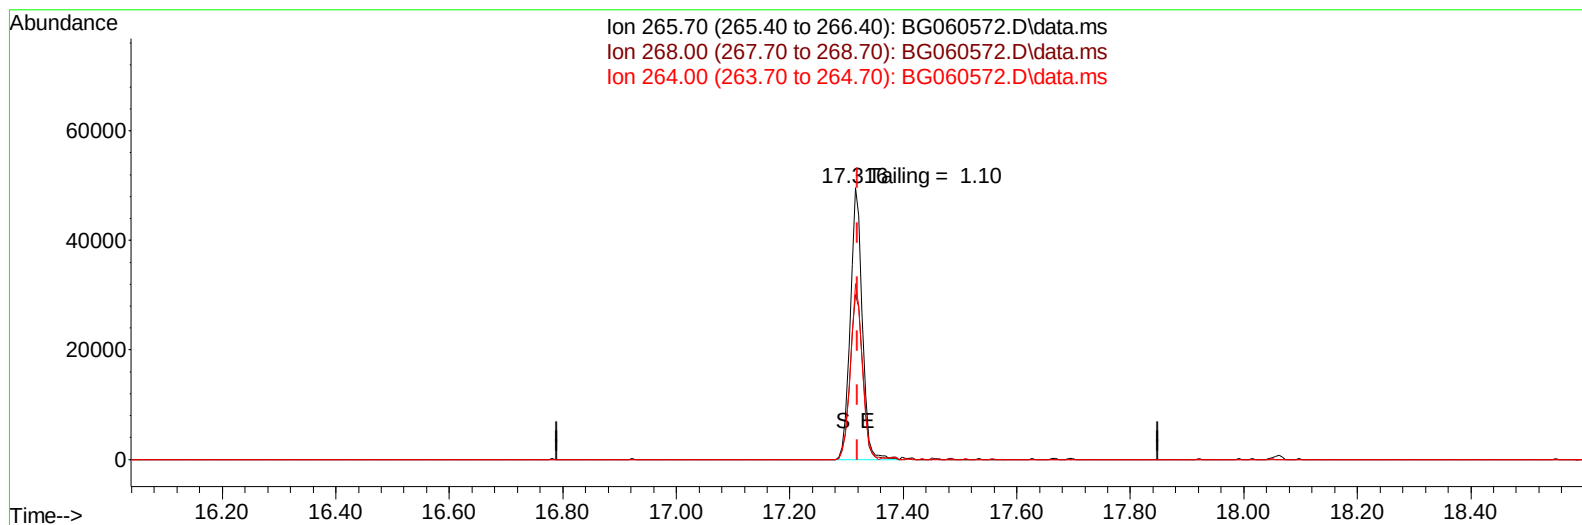

TIC: BG060572.D\data.ms

(70) Pentachlorophenol (C)




17.316min (-0.003) 9540.87 ng

response 73107

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	60.64
264.00	61.10	64.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030624\
Data File : BG060572.D
Acq On : 6 Mar 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 03:05:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 02:50:02 2024
Response via : Initial Calibration

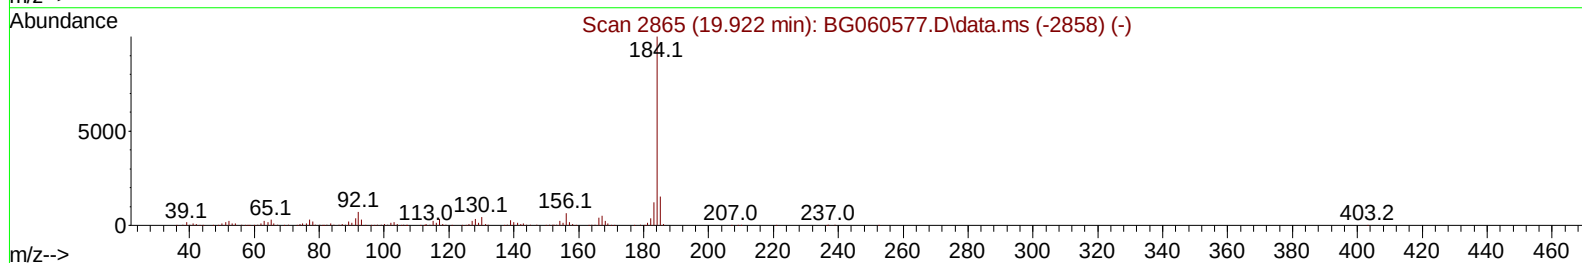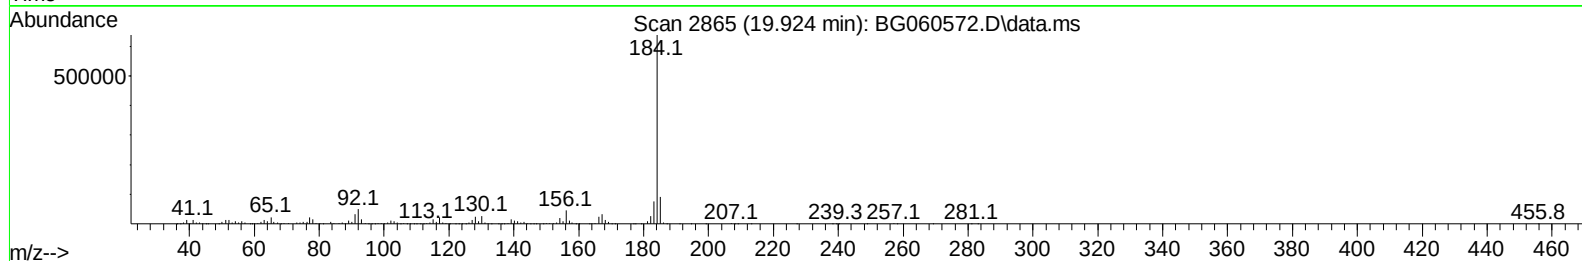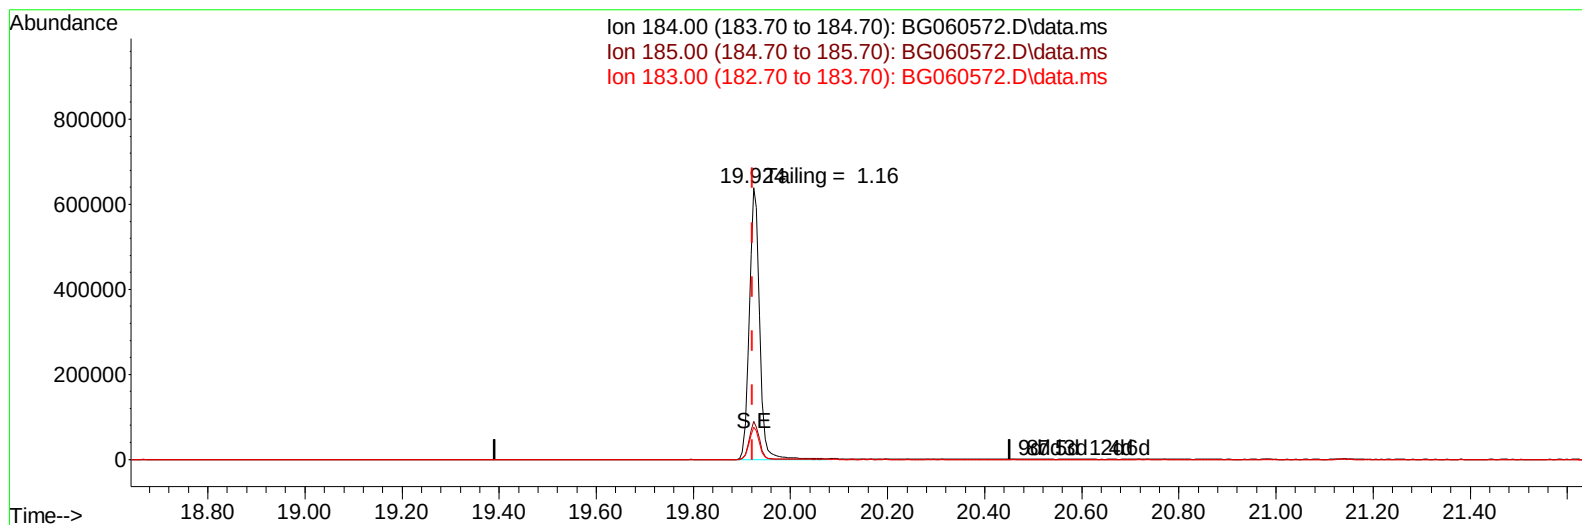

TIC: BG060572.D\data.ms

(77) Benzidine**19.924min (+ 0.003) 1564771.55 ng m****response 974084**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.15
183.00	12.10	11.92
0.00	0.00	0.00