
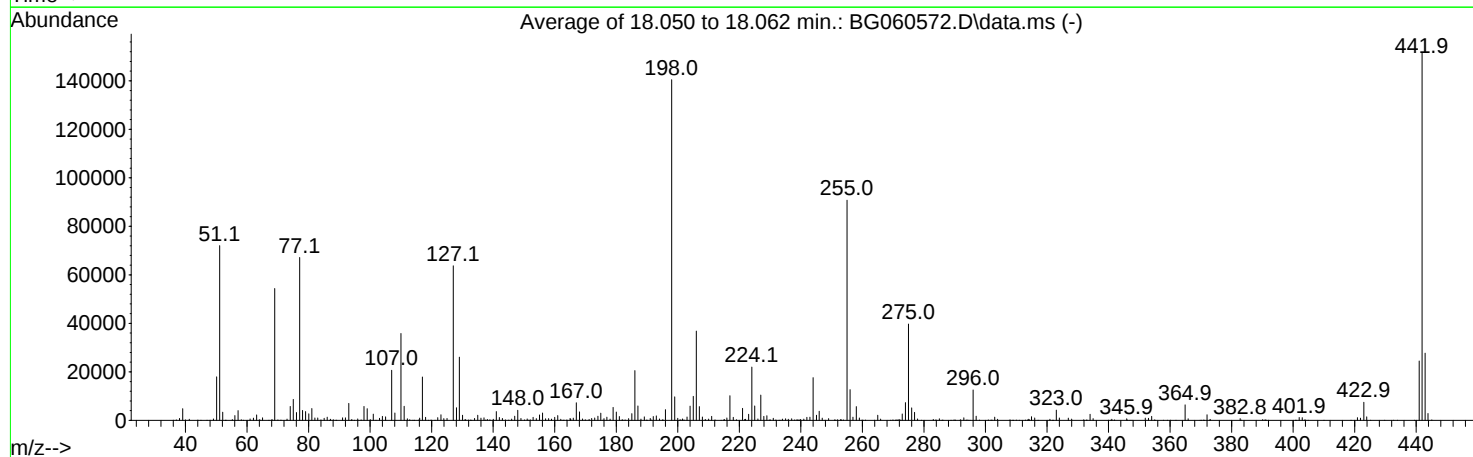


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030624\
Data File : BG060572.D
Acq On : 6 Mar 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030624.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 07 02:50:02 2024

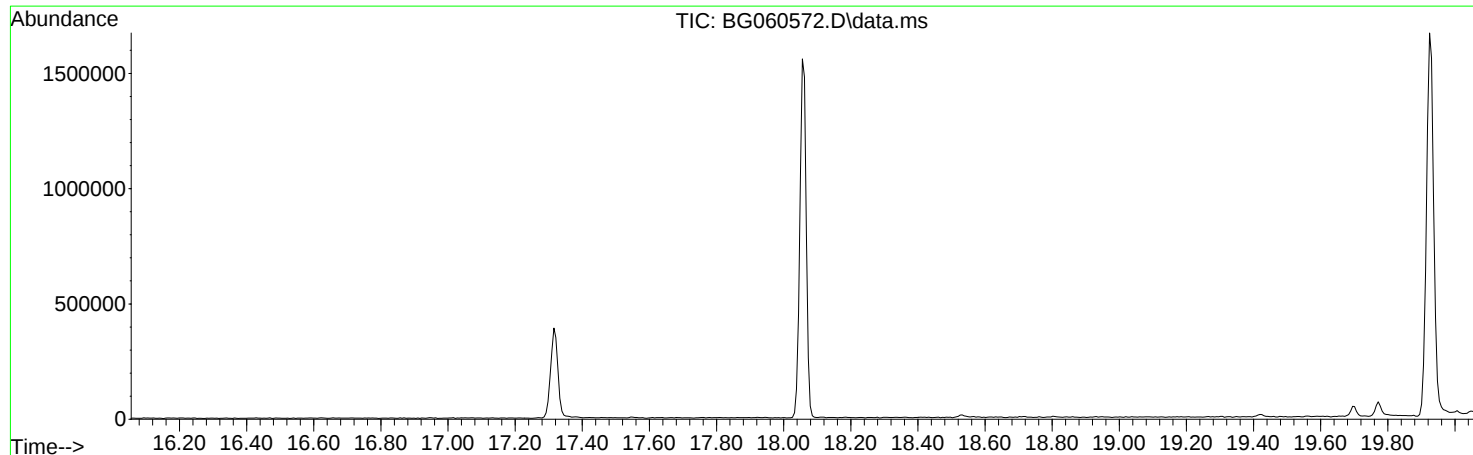




AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2539

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	51.3	72027	PASS
68	69	0.00	2	0.7	378	PASS
69	198	0.00	100	38.7	54355	PASS
70	69	0.00	2	0.4	219	PASS
127	198	10	80	45.4	63723	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	140472	PASS
199	198	5	9	6.9	9680	PASS
275	198	10	60	28.3	39725	PASS
365	198	1	100	4.5	6377	PASS
441	198	0.01	100	17.4	24488	PASS
442	442	50	100	100.0	151675	PASS
443	442	15	24	18.2	27680	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030624\
Data File : BG060572.D
Acq On : 6 Mar 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 07 03:05:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 02:50:02 2024
Response via : Initial Calibration

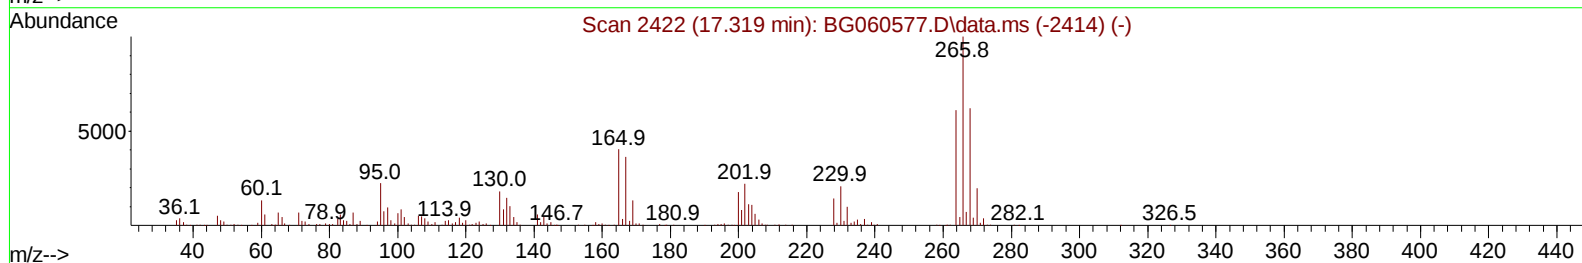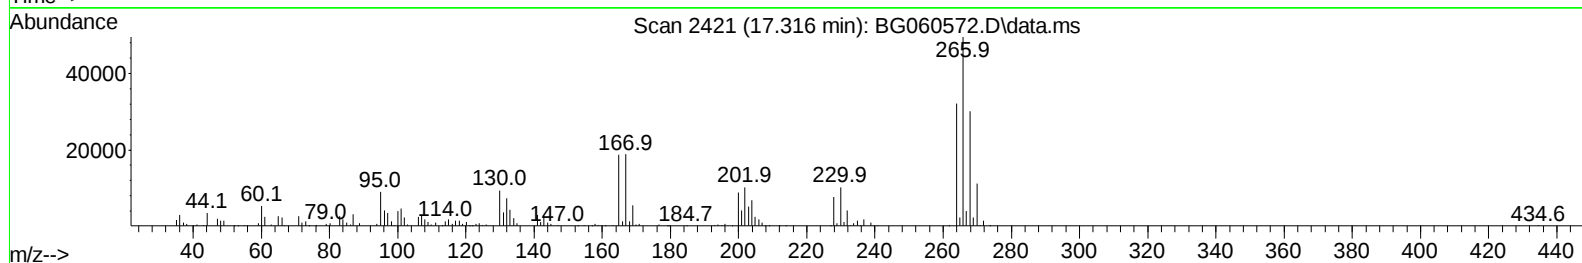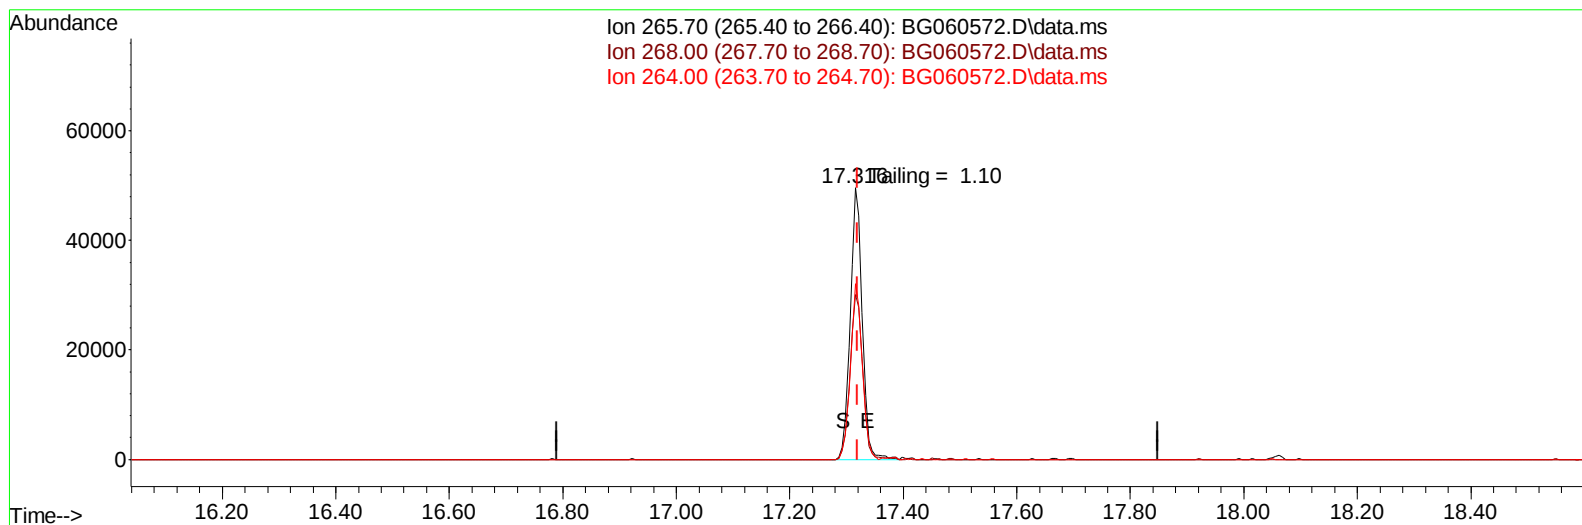

TIC: BG060572.D\data.ms

(70) Pentachlorophenol (C)

17.316min (-0.003) 9540.87 ng




response 73107

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.00	60.64
264.00	61.10	64.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030624\
Data File : BG060572.D
Acq On : 6 Mar 2024 14:31
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 07 03:05:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 07 02:50:02 2024
Response via : Initial Calibration

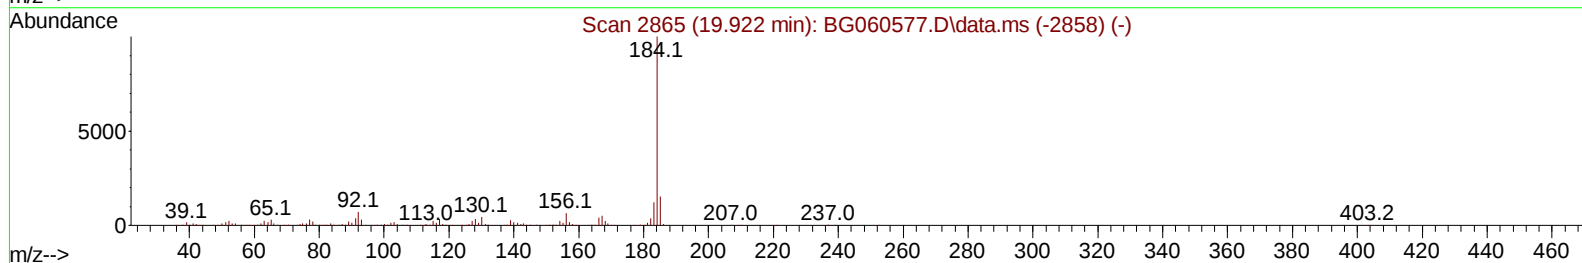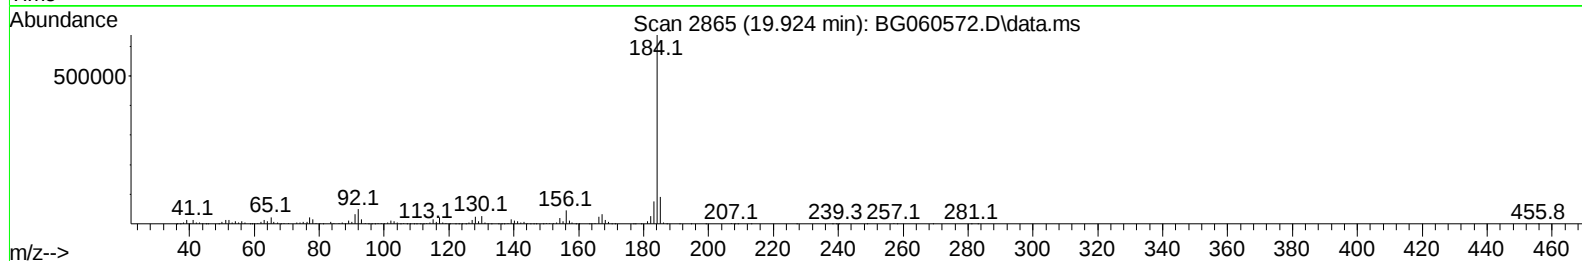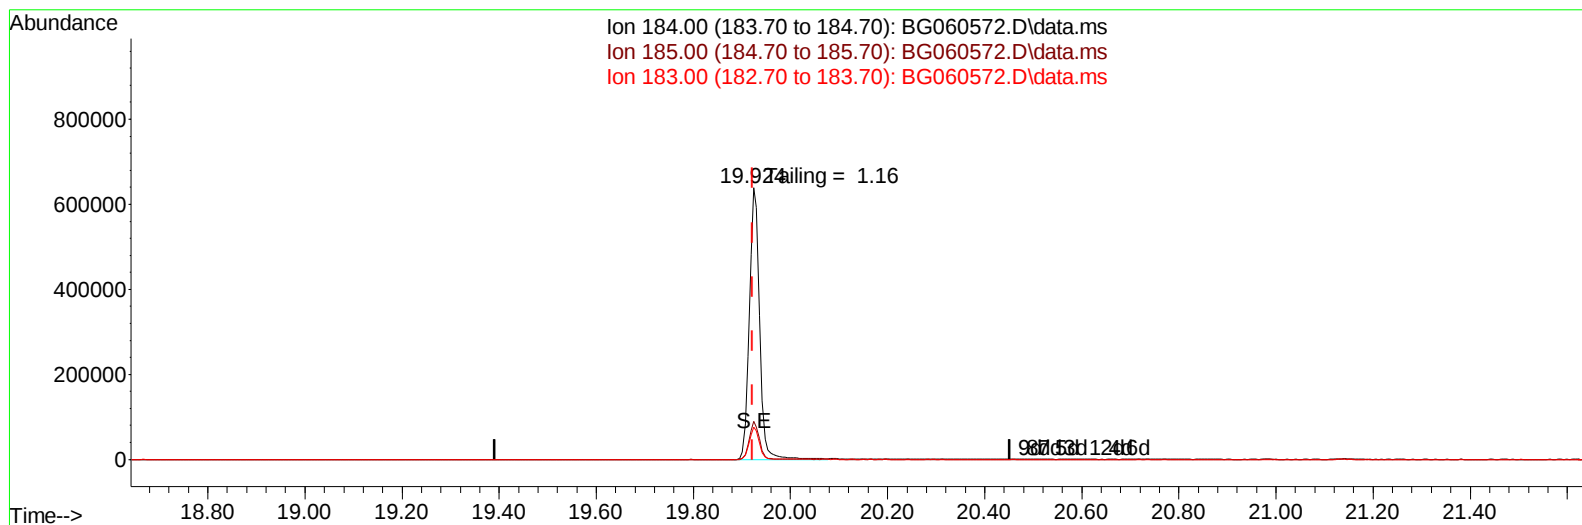

TIC: BG060572.D\data.ms

(77) Benzidine

19.924min (+ 0.003) 1564771.55 ng m

response 974084

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.15
183.00	12.10	11.92
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/6/2024	BNA_G	<u>BG060572.D</u>
Compound Name	Response	Retention Time
DDT	190787	21.14
DDD	4645	20.676
DDE	0	20.117
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4645	195432	2.38

Instrument :
BNA_G
ClientSampleId :
DFTPP