

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021332.D
 Acq On : 7 Mar 2016 10:08
 Operator : UM/SJ
 Sample : PB88659BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK59

Quant Time: Mar 07 23:57:41 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 23:58:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	8681	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	41293	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	24569	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	57617	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	61431	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	56830	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1469	6.87	ng/uL	0.00
5) Phenol-d5	7.27	99	33869	36.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	23995	39.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	24385	38.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.81	113	27109	37.34	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	13289	39.73	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	13601	38.14	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.54	165	23649	37.11	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	36873	45.63	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	82283	39.96	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	102238	39.90	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	14711	36.66	ng/ul	0.00
58) Fluorene-d10	15.72	176	72128	39.89	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	12703	30.72	ng/ul	0.00
71) Anthracene-d10	17.57	188	117136	40.88	ng/ul	0.00
79) Pyrene-d10	19.84	212	130634	42.01	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	125816	41.01	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.81	70	770	1.01	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021332.D
Acq On : 7 Mar 2016 10:08
Operator : UM/SJ
Sample : PB88659BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK59

Quant Time: Mar 07 23:57:41 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 23:58:06 2016
Response via : Initial Calibration

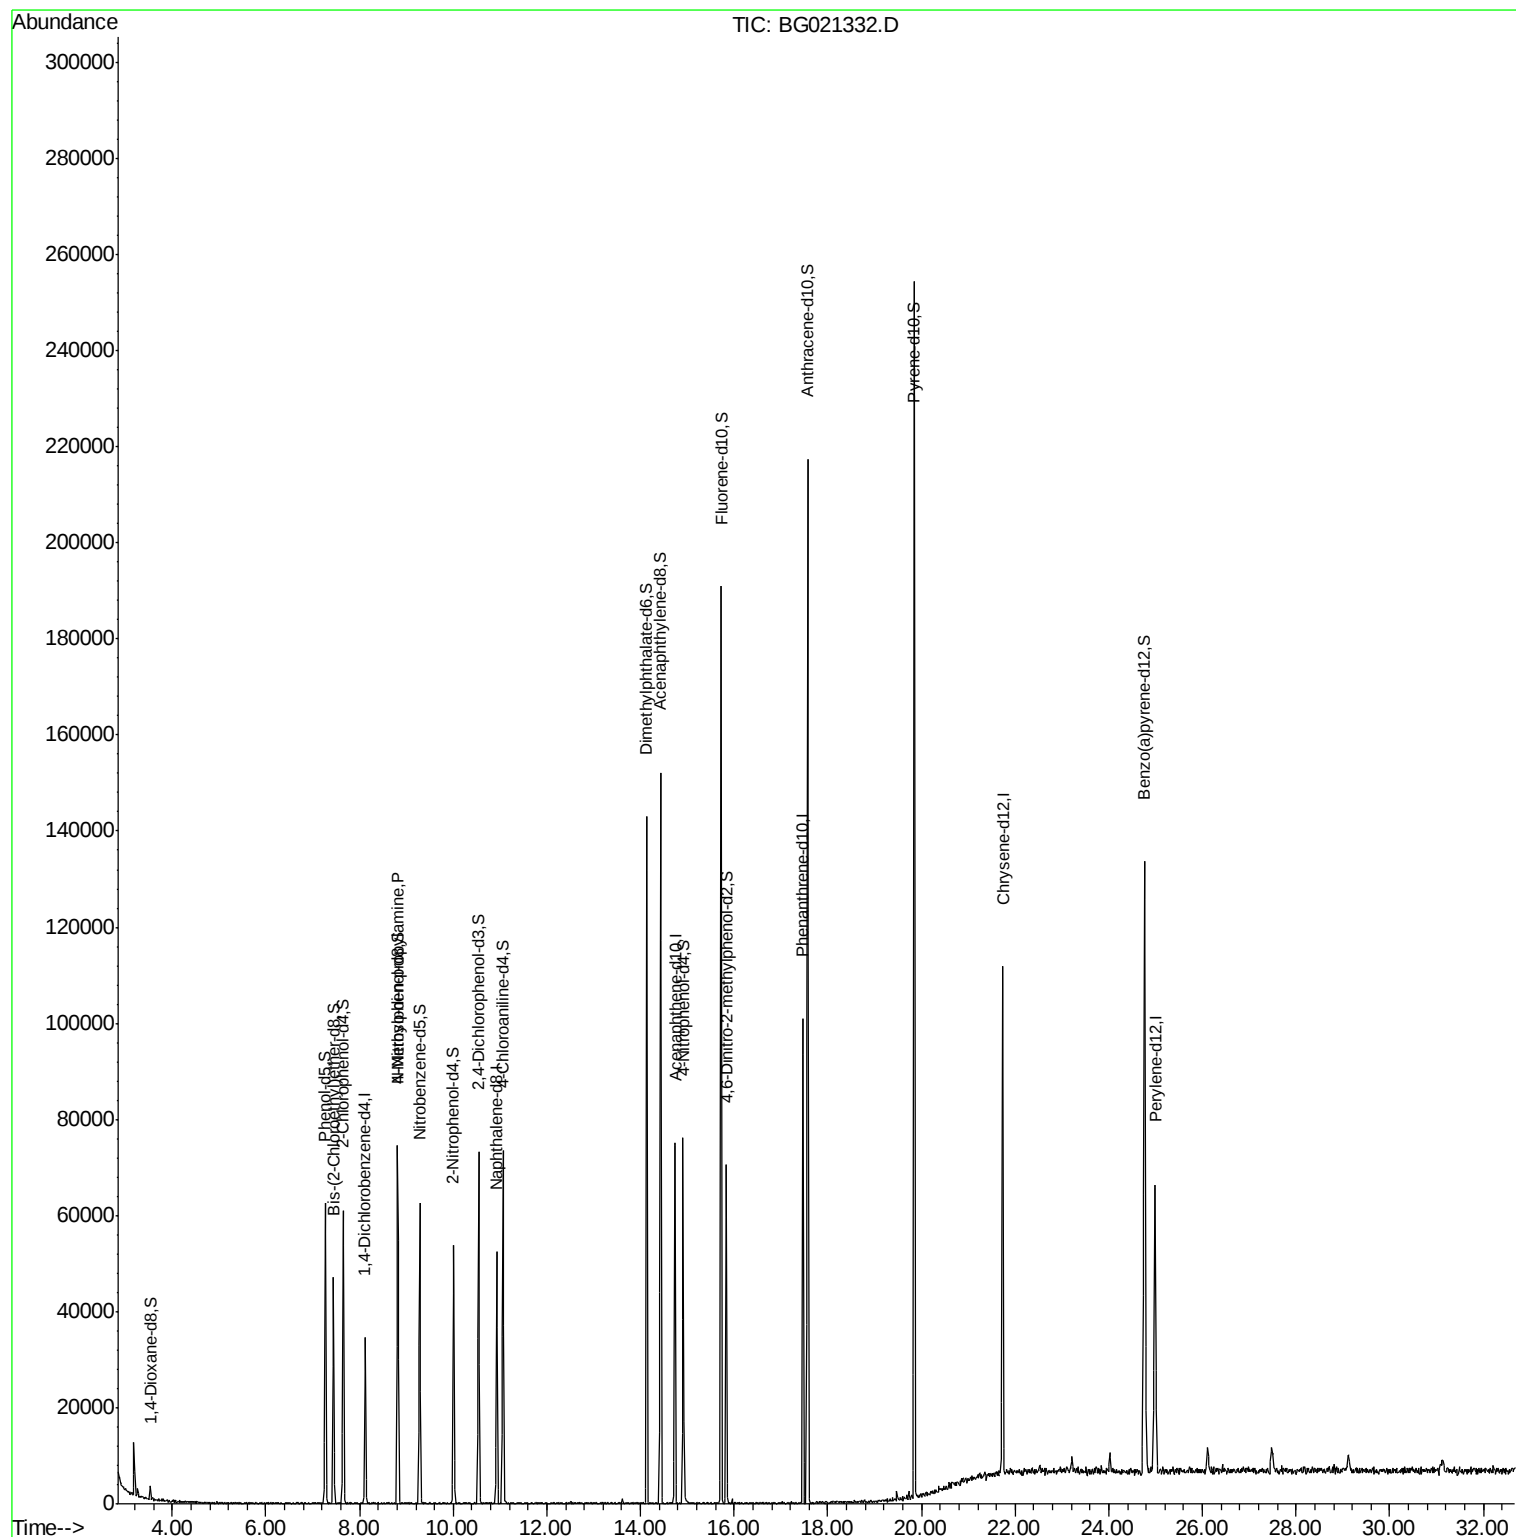

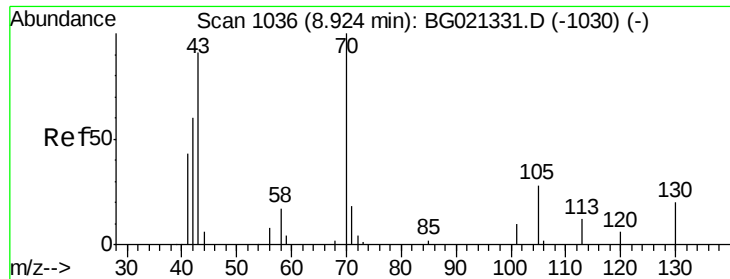

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.01 ng/ul
 RT: 8.81 min Scan# 1017
 Delta R.T. -0.11 min
 Lab File: BG021332.D
 Acq: 7 Mar 2016 10:08

Instrument :
 BNA_G
 ClientSampleId :
 SBLK59

Tgt Ion:	70	Resp:	770
Ion	Ratio	Lower	Upper
70	100		
42	450.0	45.7	68.5#
101	0.0	5.7	8.5#
130	0.0	15.7	23.5#

