

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021334.D
 Acq On : 7 Mar 2016 11:27
 Operator : UM/SJ
 Sample : H1625-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFF0

Quant Time: Mar 07 23:57:55 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 23:58:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9509	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	45807	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	27369	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	64407	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	69486	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	63968	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1172	5.01	ng/uL	0.00
5) Phenol-d5	7.27	99	28967	28.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	22273	33.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	21764	30.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	23105	29.06	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	11702	31.54	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	12593	31.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	21580	30.53	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	33081	36.90	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	76779	33.48	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	97032	34.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	13646	30.52	ng/ul	0.00
58) Fluorene-d10	15.72	176	68975	34.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	12601	27.26	ng/ul	0.00
71) Anthracene-d10	17.57	188	112365	35.08	ng/ul	0.00
79) Pyrene-d10	19.84	212	126596	35.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	121953	35.32	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	28945	11.73	ng/ul#	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021334.D
Acq On : 7 Mar 2016 11:27
Operator : UM/SJ
Sample : H1625-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFF0

Quant Time: Mar 07 23:57:55 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 23:58:06 2016
Response via : Initial Calibration

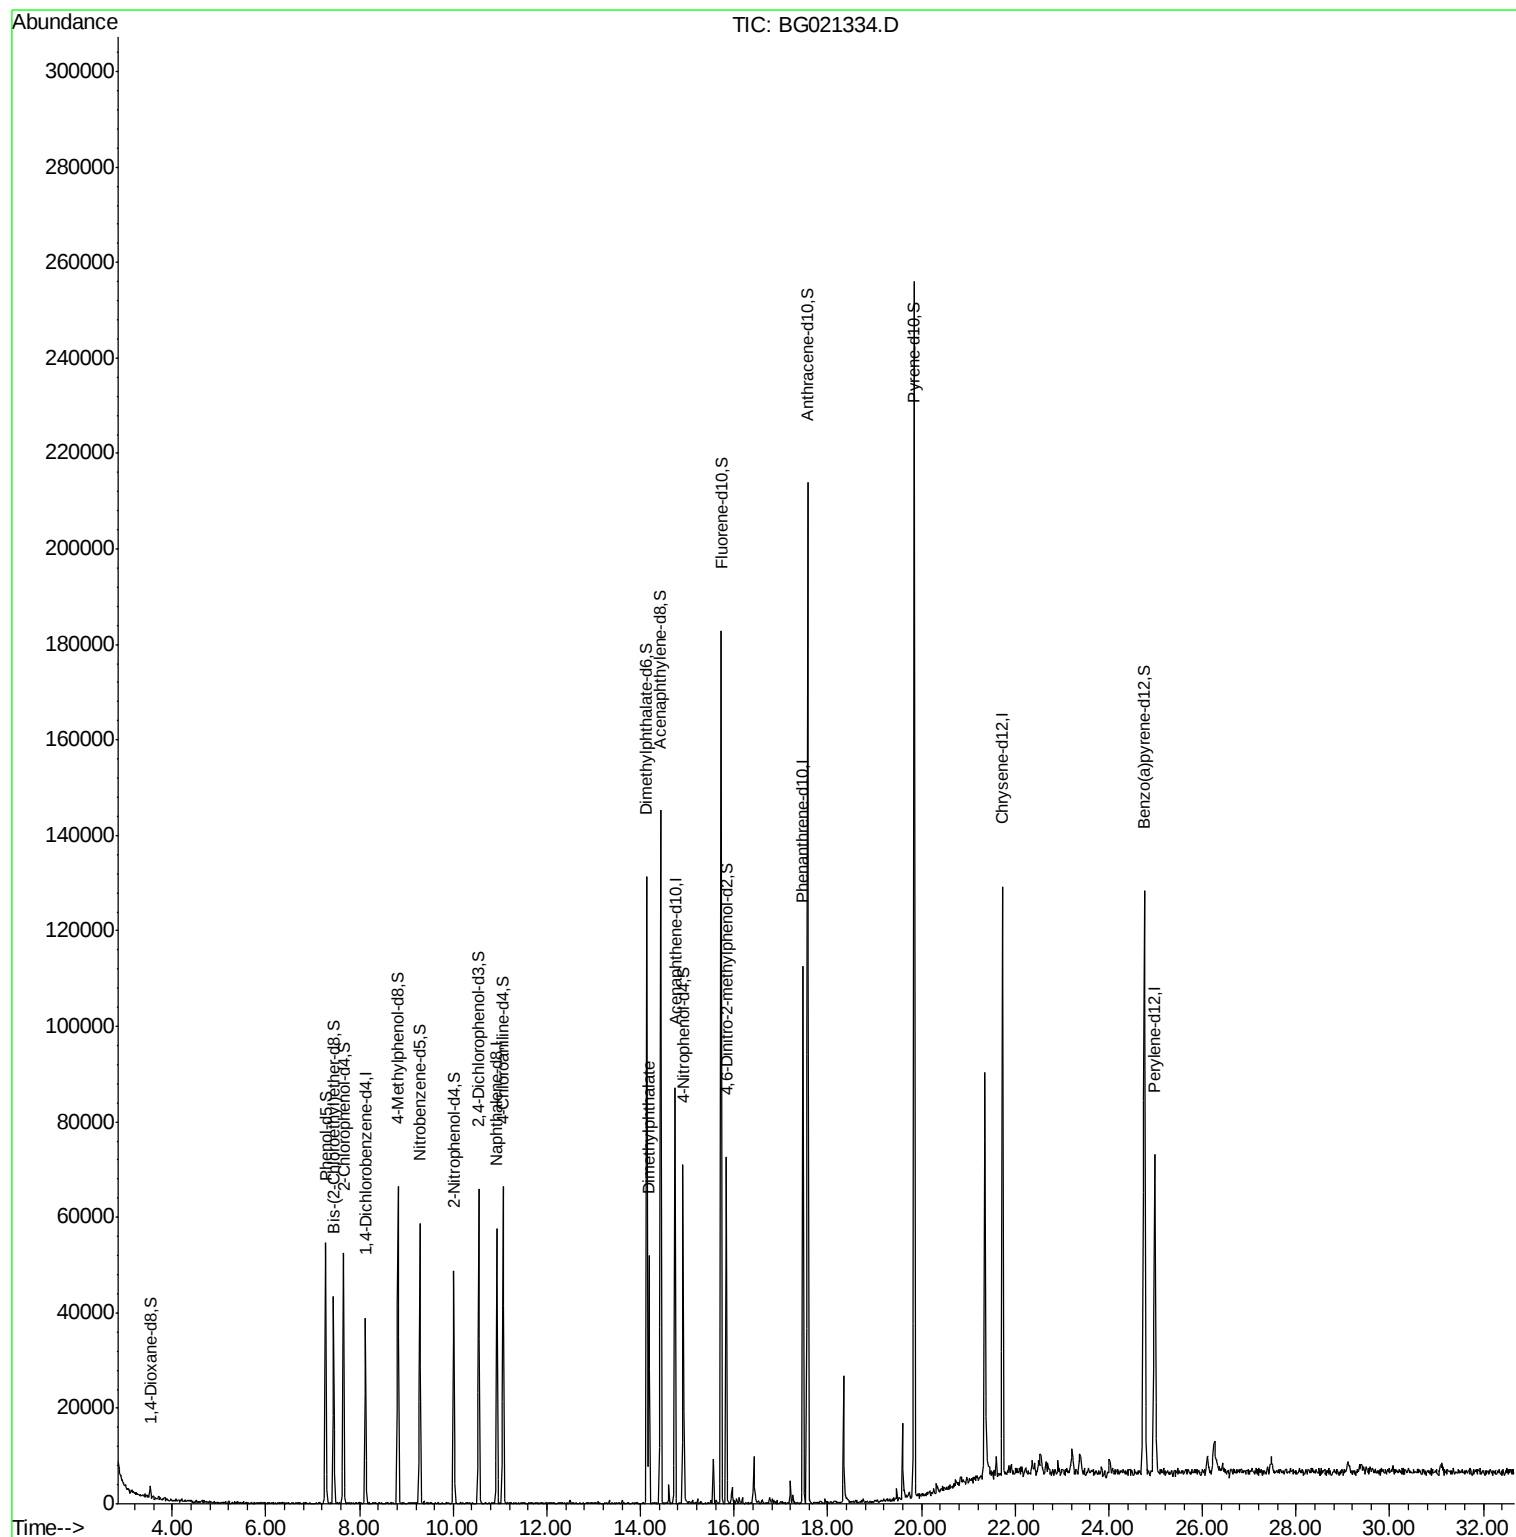

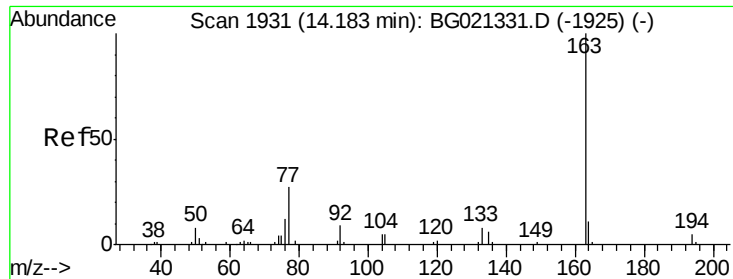

#45

Dimethylphthalate

Concen: 11.73 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BG021334.D


Acq: 7 Mar 2016 11:27

Instrument :

BNA_G

ClientSampleId :

JHFF0

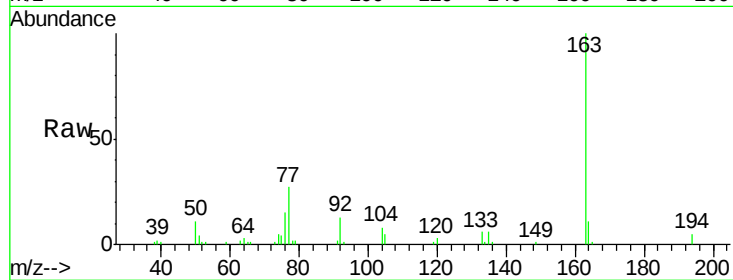

Tgt Ion:	163	Resp:	28945
Ion	Ratio	Lower	Upper
163	100		
194	4.6	2.8	4.2#
164	10.5	8.2	12.2

