

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021338.D
 Acq On : 7 Mar 2016 14:04
 Operator : UM/SJ
 Sample : H1625-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFF2

Quant Time: Mar 07 23:58:33 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 23:58:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10398	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	49504	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	29818	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.57	188	131025	20.00	ng/ul	0.10
78) Chrysene-d12	21.73	240	72890	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	67738	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1254	4.90	ng/uL	0.00
5) Phenol-d5	7.27	99	33663	30.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	24861	33.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	25385	33.04	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	23487	27.01	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	13543	33.77	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	14769	34.55	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	25606	33.52	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	35682	36.83	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	92269	36.93	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	114668	36.88	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15673	32.18	ng/ul	0.00
58) Fluorene-d10	15.72	176	82873	37.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	15274	16.24	ng/ul	0.00
71) Anthracene-d10	17.57	188	131025	20.11	ng/ul	0.00
79) Pyrene-d10	19.84	212	144259	39.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	139031	38.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	37834	14.07	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021338.D
Acq On : 7 Mar 2016 14:04
Operator : UM/SJ
Sample : H1625-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFF2

Quant Time: Mar 07 23:58:33 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 23:58:06 2016
Response via : Initial Calibration

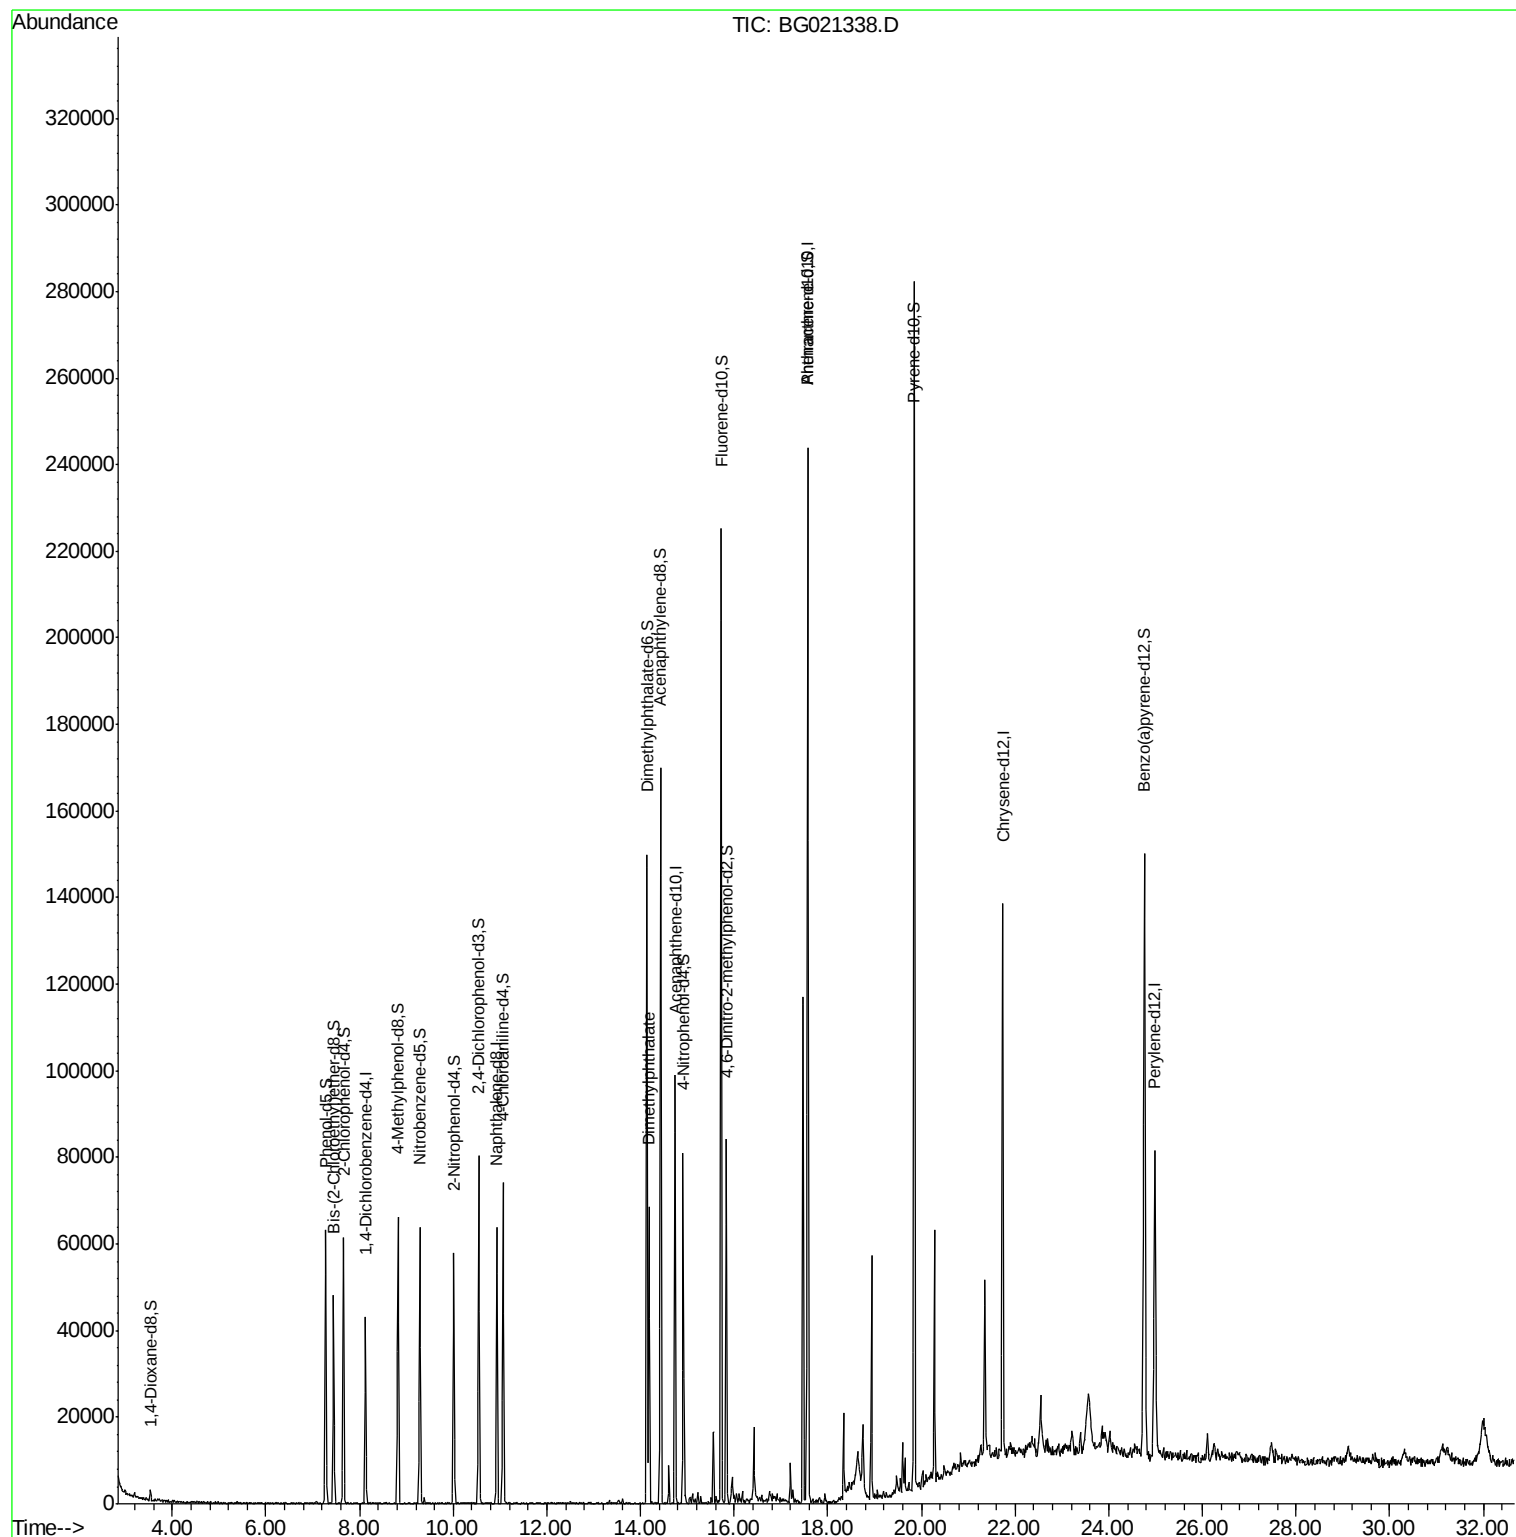

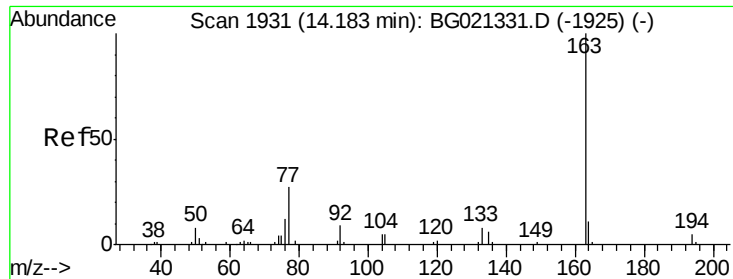

#45

Dimethylphthalate

Concen: 14.07 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.01 min

Lab File: BG021338.D

Acq: 7 Mar 2016 14:04

Instrument :

BNA_G

ClientSampleId :

JHFF2


Tgt Ion:163 Resp: 37834

Ion Ratio Lower Upper

163 100

194 3.9 2.8 4.2

164 10.7 8.2 12.2

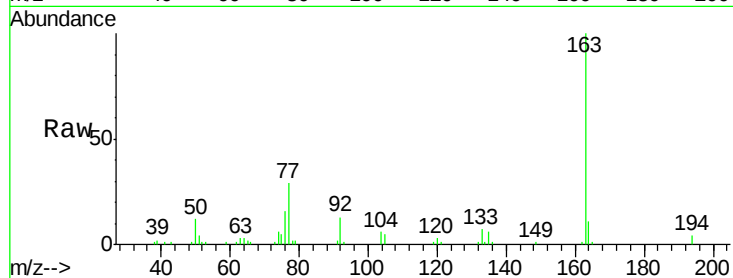

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

