

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021341.D
 Acq On : 7 Mar 2016 16:03
 Operator : UM/SJ
 Sample : H1625-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFG2

Quant Time: Mar 07 23:58:56 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 23:58:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	11883	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	55256	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	32088	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	72887	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	78330	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	73204	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	653	2.23	ng/uL	0.00
5) Phenol-d5	7.27	99	19723	15.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	13732	16.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	14717	16.76	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	14185	14.27	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	7447	16.64	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	7556	15.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	13951	16.36	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	13503	12.49	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	43986	16.36	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	60431	18.06	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	5279	10.07	ng/ul	0.00
58) Fluorene-d10	15.72	176	42848	18.14	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	4261	8.15	ng/ul	0.00
71) Anthracene-d10	17.57	188	66089	18.23	ng/ul	0.00
79) Pyrene-d10	19.84	212	75228	18.97	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	72554	18.36	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	20681	7.15	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021341.D
Acq On : 7 Mar 2016 16:03
Operator : UM/SJ
Sample : H1625-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFG2

Quant Time: Mar 07 23:58:56 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 23:58:06 2016
Response via : Initial Calibration

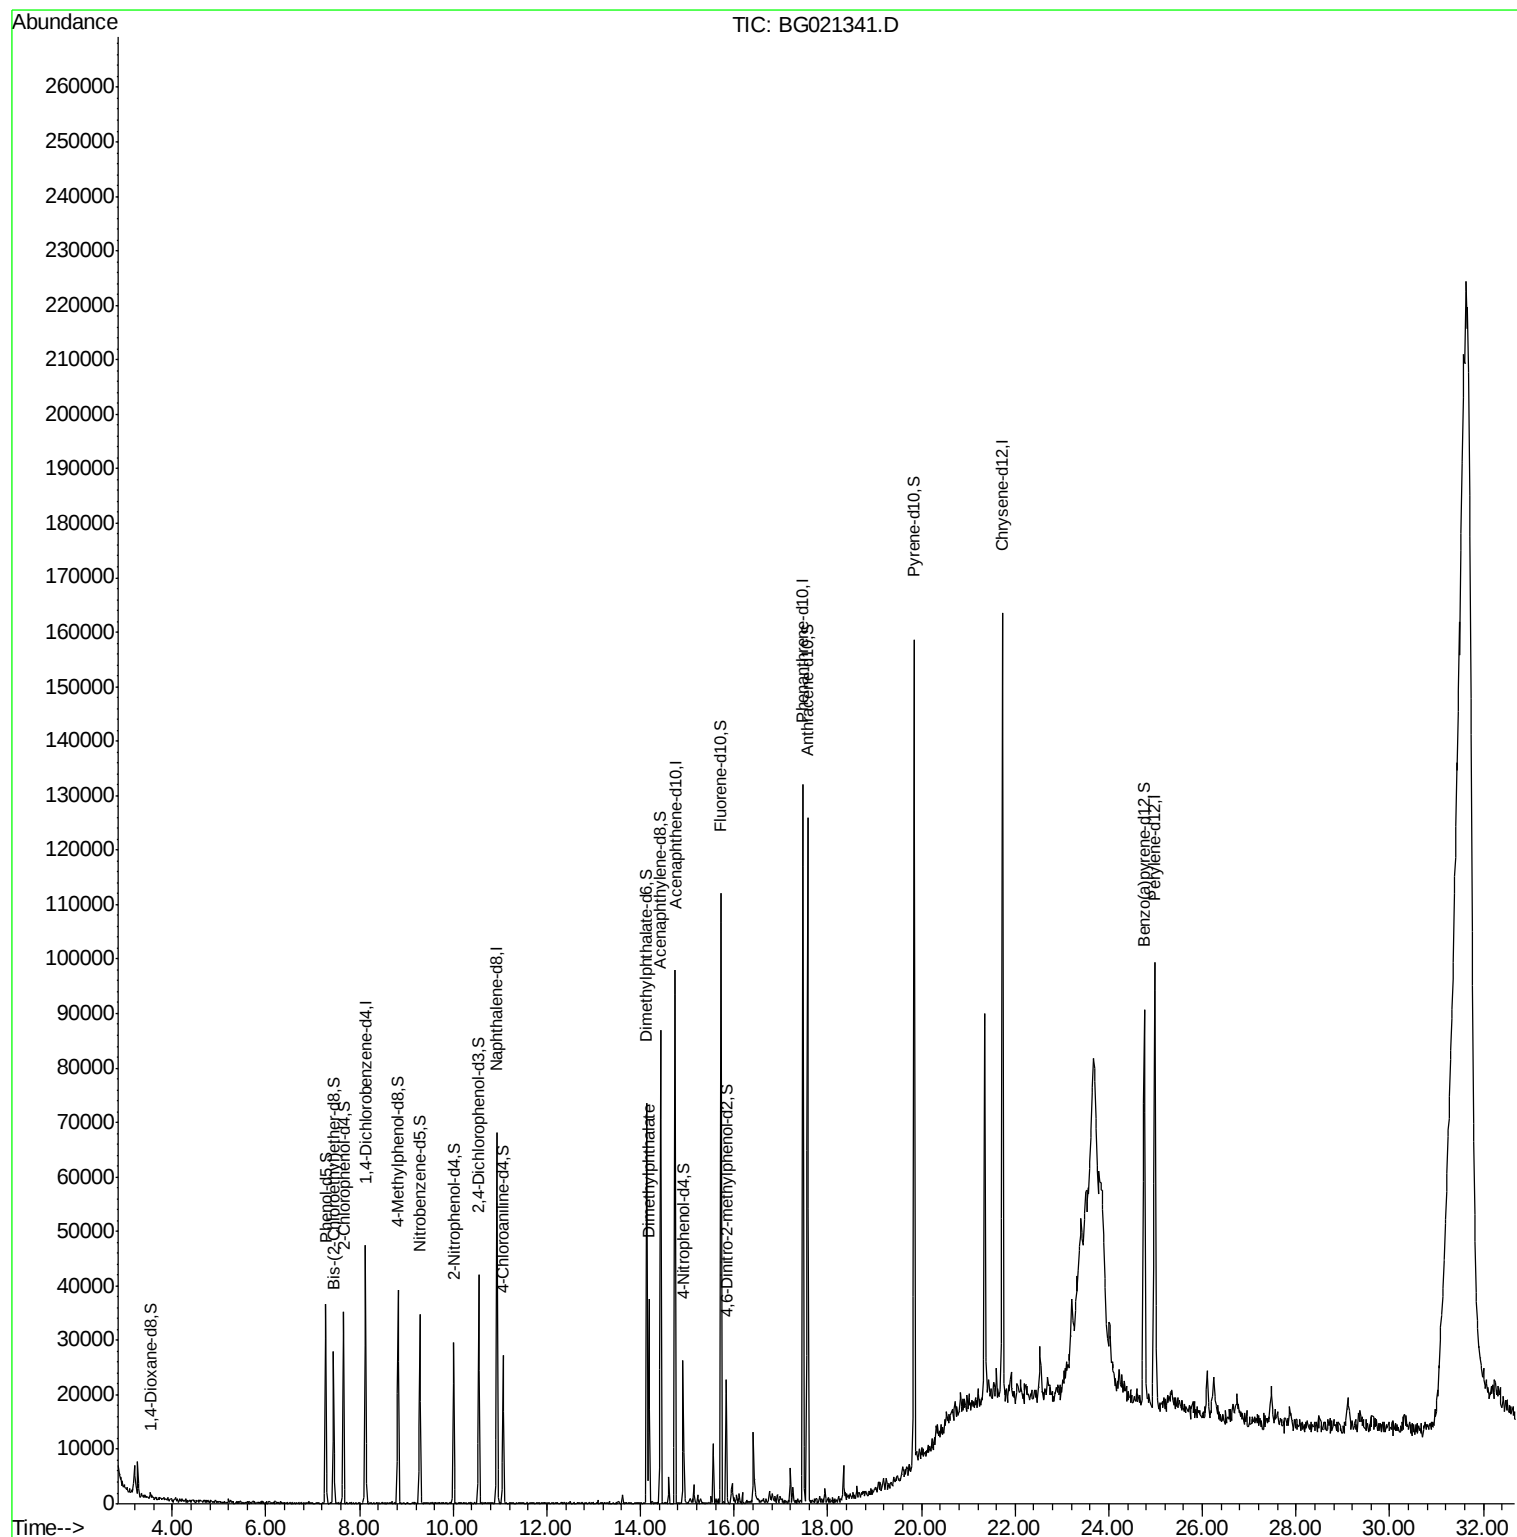


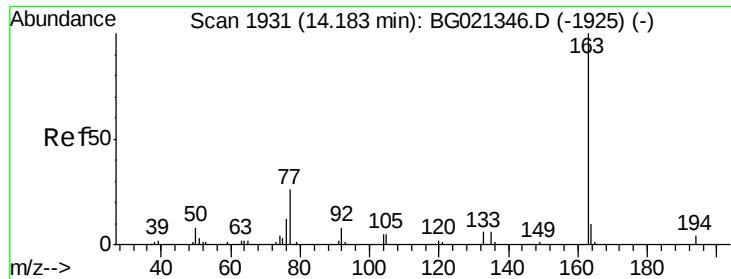

#45
 Dimethylphthalate
 Concen: 7.15 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021341.D
 Acq: 7 Mar 2016 16:03

Instrument :
 BNA_G
 ClientSampleId :
 JHFG2

Tgt Ion:163 Resp: 20681
 Ion Ratio Lower Upper
 163 100
 194 4.3 2.8 4.2#
 164 9.7 8.2 12.2

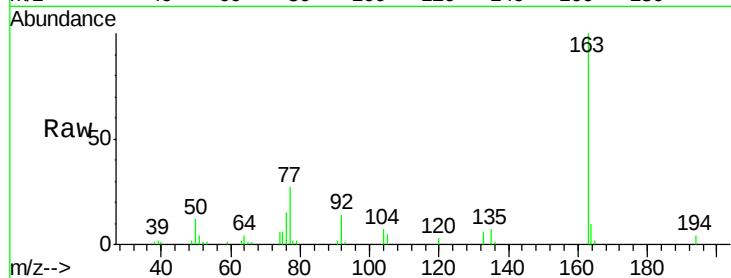

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

