

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021344.D
 Acq On : 7 Mar 2016 18:01
 Operator : UM/SJ
 Sample : H1625-19
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFM6

Quant Time: Mar 07 23:59:20 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 07 23:58:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9827	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	48215	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	28472	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	66029	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	69095	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	65289	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1158	4.79	ng/uL	0.00
5) Phenol-d5	7.27	99	29256	28.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	19923	28.71	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	21183	29.17	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	24171	29.41	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	11360	29.09	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	11788	28.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	20967	28.18	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	26094	27.65	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	66353	27.81	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	87606	29.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	11228	24.14	ng/ul	0.00
58) Fluorene-d10	15.72	176	62088	29.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	9699	20.47	ng/ul	0.00
71) Anthracene-d10	17.57	188	96650	29.43	ng/ul	0.00
79) Pyrene-d10	19.84	212	108063	30.90	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	102585	29.11	ng/ul	0.00


Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	24713	9.63 ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021344.D
Acq On : 7 Mar 2016 18:01
Operator : UM/SJ
Sample : H1625-19
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH6

Quant Time: Mar 07 23:59:20 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 07 23:58:06 2016
Response via : Initial Calibration

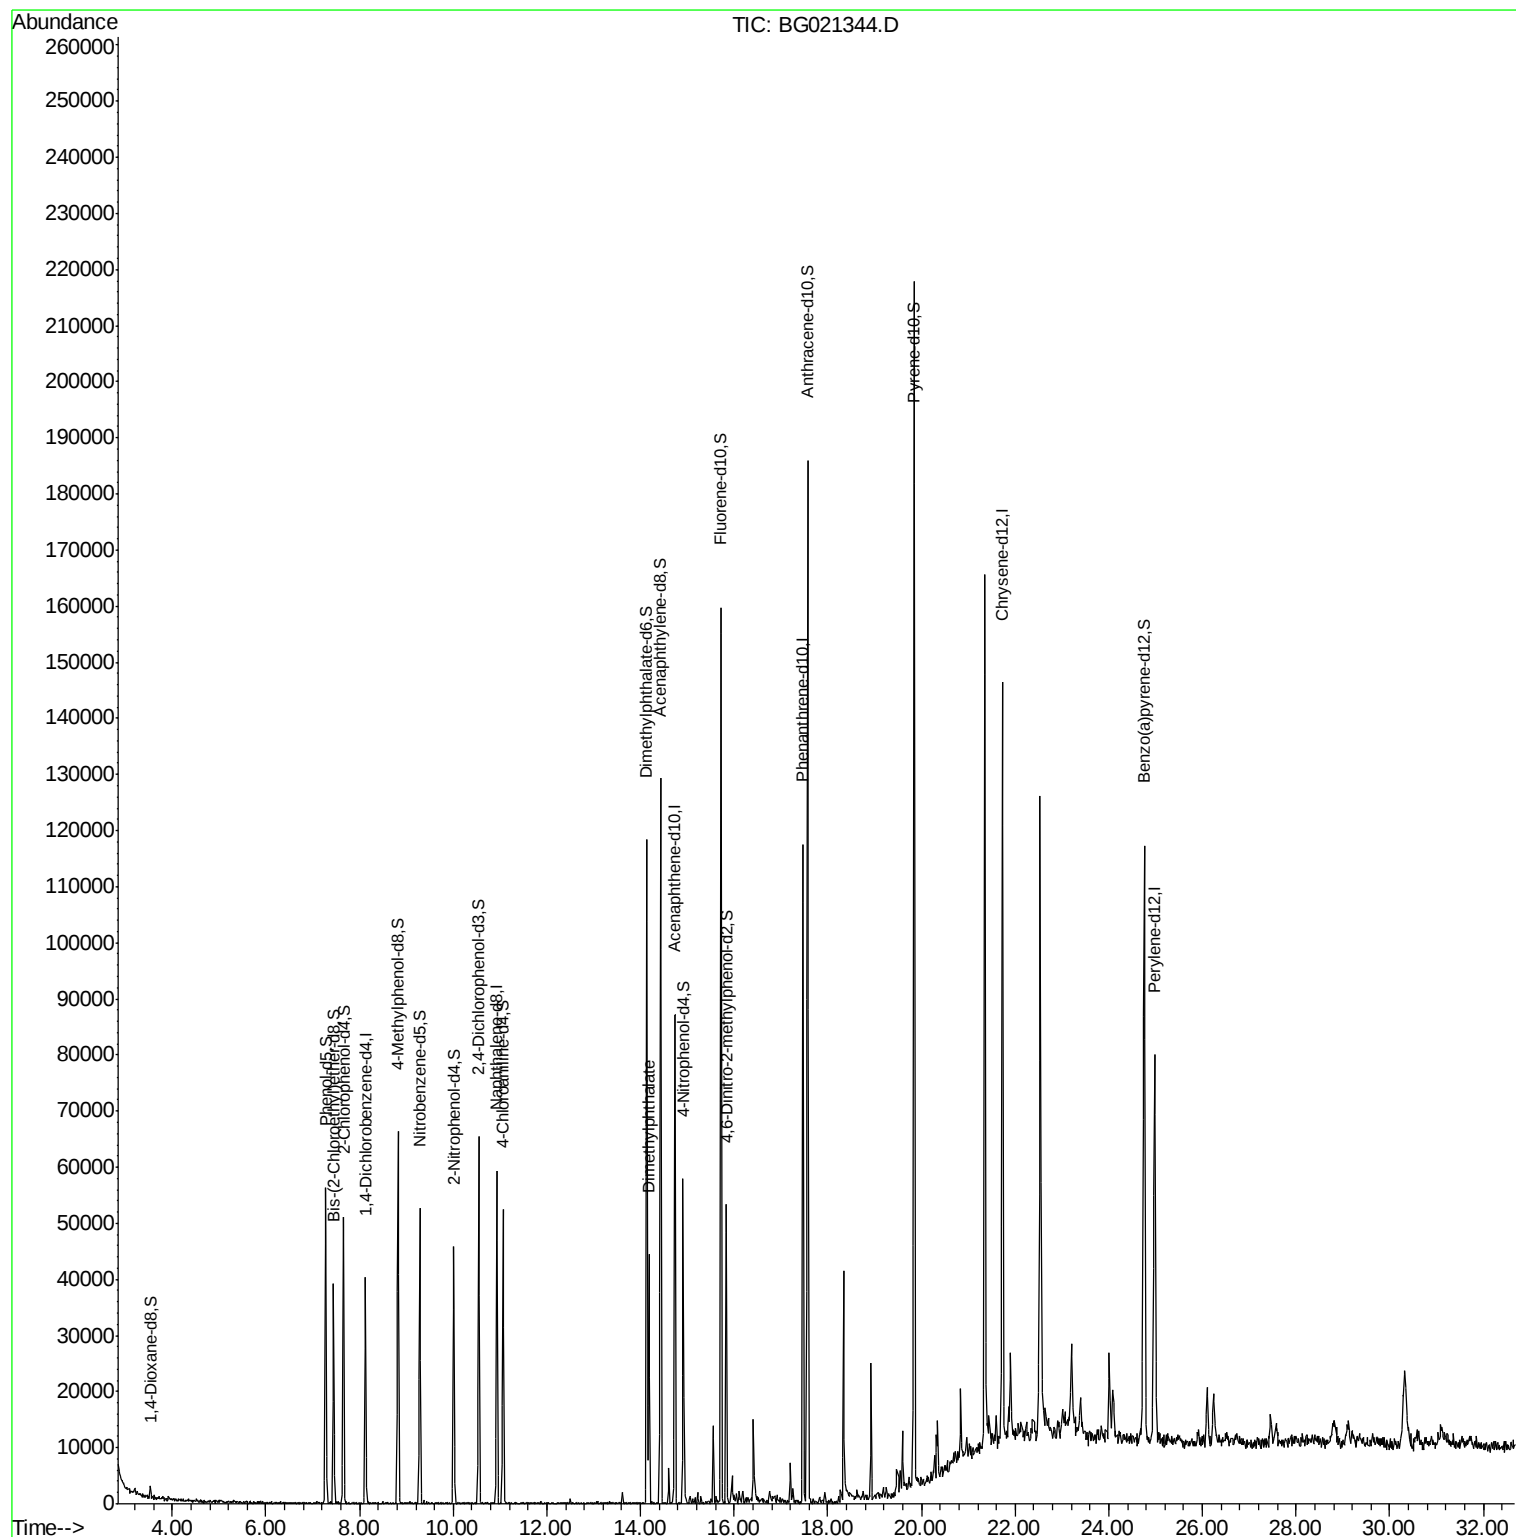


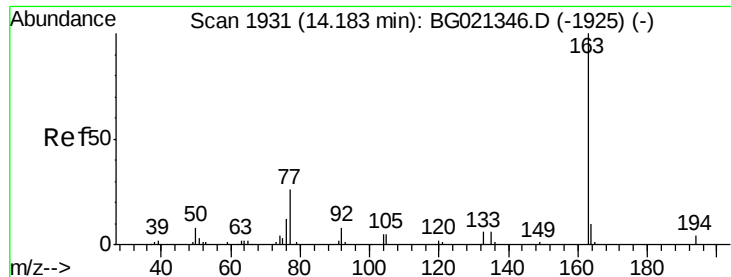

#45
 Dimethylphthalate
 Concen: 9.63 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021344.D
 Acq: 7 Mar 2016 18:01

Instrument :
 BNA_G
 ClientSampleId :
 JHFM6

Tgt Ion:163 Resp: 24713
 Ion Ratio Lower Upper
 163 100
 194 4.4 2.8 4.2#
 164 10.8 8.2 12.2

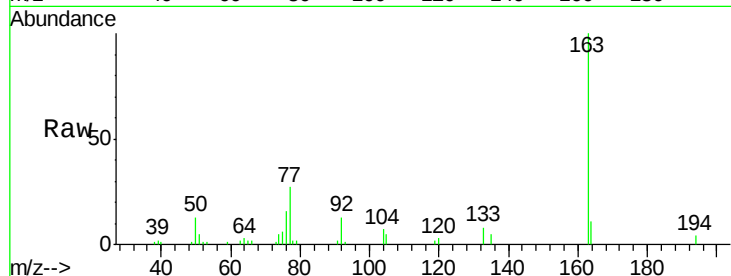

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

