

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021350.D
 Acq On : 7 Mar 2016 22:37
 Operator : UM/SJ
 Sample : H1625-12 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFG9

Manual Integrations
 APPROVED

Sohil
 3/8/2016 2:43:39 PM

Quant Time: Mar 08 01:09:56 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 08 00:45:15 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	10356	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	49655	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	28516	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	65197m	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	68466	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	65629	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	0.00	96	0	0.00	ng/uL	
5) Phenol-d5	7.28	99	3027	2.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	2454	3.36	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	2105	2.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	2139	2.47	ng/ul	0.00
19) Nitrobenzene-d5	9.28	128	1196	2.97	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	1123	2.62	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	2103	2.74	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	2246	2.31	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	7645	3.20	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	10387	3.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	413	0.89	ng/ul	0.00
58) Fluorene-d10	15.72	176	7237	3.45	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	479	1.02	ng/ul	0.00
71) Anthracene-d10	17.57	188	11166	3.44	ng/ul	0.00
79) Pyrene-d10	19.84	212	12641	3.65	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	12208	3.45	ng/ul	0.00

Target Compounds					Qvalue
45) Dimethylphthalate	14.18	163	2771	1.08 ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021350.D
Acq On : 7 Mar 2016 22:37
Operator : UM/SJ
Sample : H1625-12 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
JHFG9

Manual Integrations
APPROVED

Sohil
3/8/2016 2:43:39 PM

Quant Time: Mar 08 01:09:56 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 08 00:45:15 2016
Response via : Initial Calibration

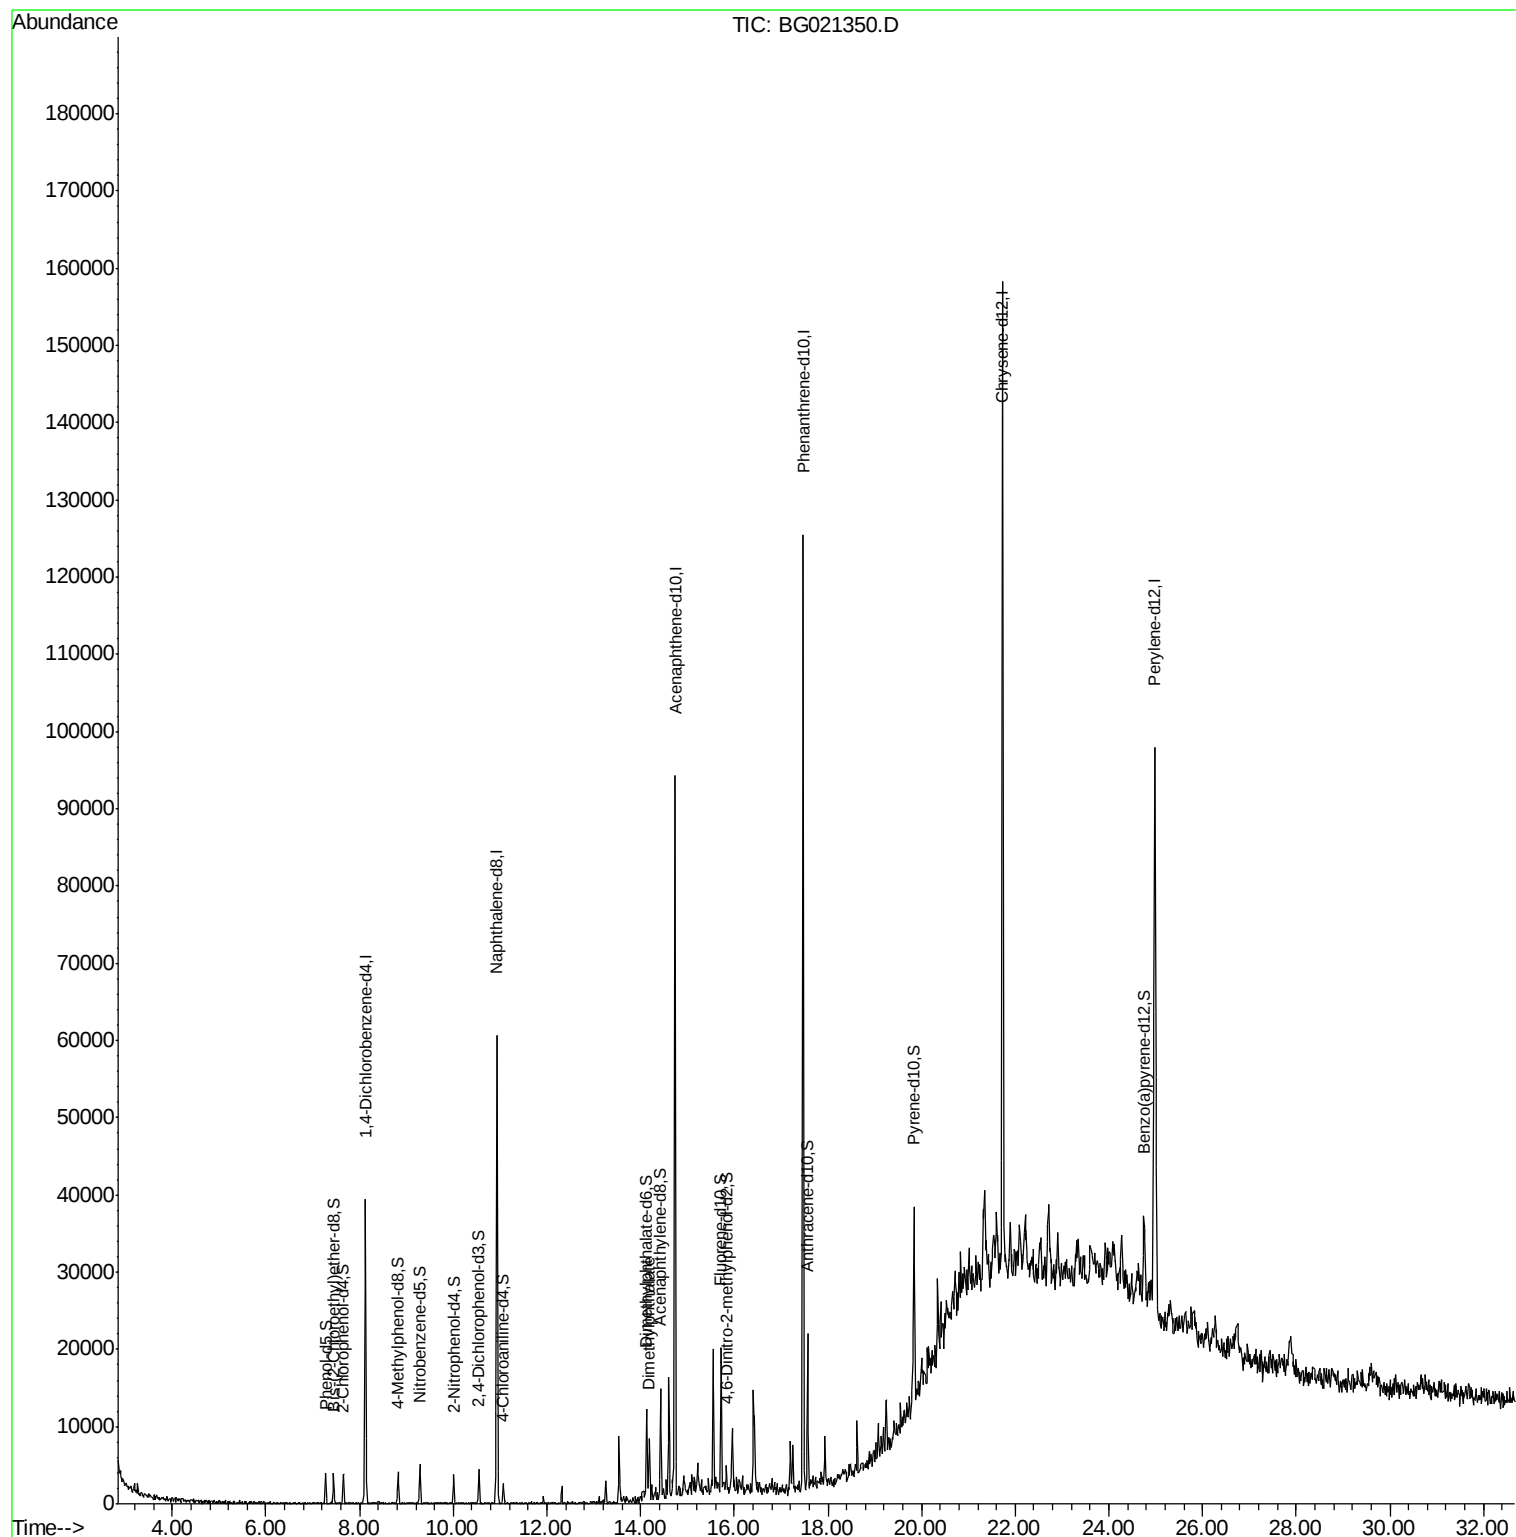

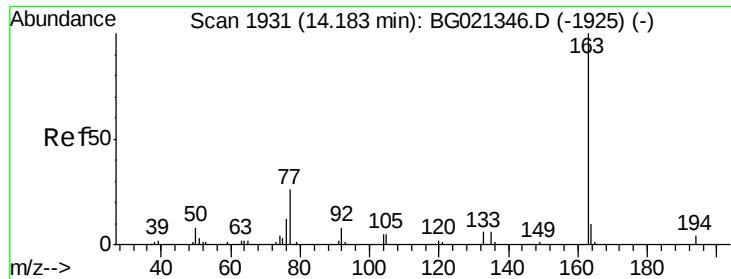

#45
 Dimethylphthalate
 Concen: 1.08 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021350.D
 Acq: 7 Mar 2016 22:37

Instrument :
 BNA_G
 ClientSampleId :
 JHFG9

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	2771		
194	0.0	2.8	4.2#	
164	8.9	8.2	12.2	

Manual Integrations
 APPROVED

Sohil
 3/8/2016 2:43:39 PM

