

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021353.D
 Acq On : 8 Mar 2016 00:35
 Operator : UM/SJ
 Sample : H1625-16 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.060	36	38	40	rBV	709	533	0.26%	0.050%
2	3.183	58	59	66	rVB3	1378	1679	0.82%	0.159%
3	3.230	66	67	70	rBV3	429	487	0.24%	0.046%
4	3.336	83	85	86	rBV2	749	495	0.24%	0.047%
5	3.389	93	94	98	rVB2	592	555	0.27%	0.052%
6	3.424	98	100	102	rBV2	452	488	0.24%	0.046%
7	3.548	118	121	125	rVB2	369	388	0.19%	0.037%
8	3.712	146	149	151	rVB2	373	430	0.21%	0.041%
9	3.742	151	154	156	rBV	286	386	0.19%	0.036%
10	4.182	228	229	231	rBV	615	415	0.20%	0.039%
11	4.341	254	256	259	rVV	505	594	0.29%	0.056%
12	4.523	285	287	291	rBV	240	397	0.19%	0.037%
13	4.558	291	293	294	rVB	686	403	0.20%	0.038%
14	4.576	294	296	299	rBV	477	595	0.29%	0.056%
15	4.682	311	314	316	rVV	428	470	0.23%	0.044%
16	4.699	316	317	321	rVB	401	494	0.24%	0.047%
17	4.799	333	334	337	rVB	556	501	0.24%	0.047%
18	4.911	348	353	355	rBV2	371	660	0.32%	0.062%
19	5.075	378	381	385	rBB	225	410	0.20%	0.039%
20	5.140	391	392	396	rBB	367	392	0.19%	0.037%
21	5.857	512	514	516	rBV	366	406	0.20%	0.038%
22	7.279	752	756	761	rVB	2022	3112	1.52%	0.294%
23	7.443	781	784	789	rBB	2163	2970	1.45%	0.280%
24	7.661	816	821	824	rBB	1990	2850	1.39%	0.269%
25	8.125	894	900	907	rBB	43386	69675	33.92%	6.578%
26	8.824	1014	1019	1024	rBB2	2113	3033	1.48%	0.286%
27	9.294	1093	1099	1103	rBV3	2399	4201	2.05%	0.397%
28	10.011	1218	1221	1224	rBB2	1381	1840	0.90%	0.174%
29	10.545	1309	1312	1317	rBB2	1910	3184	1.55%	0.301%
30	10.933	1371	1378	1386	rBB	62866	109424	53.27%	10.331%
31	11.074	1398	1402	1406	rBB	1036	1163	0.57%	0.110%
32	14.129	1918	1922	1927	rBV	5293	7213	3.51%	0.681%
33	14.176	1927	1930	1934	rVB	1348	1529	0.74%	0.144%
34	14.429	1968	1973	1978	rBB2	6195	8822	4.30%	0.833%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021353.D
 Acq On : 8 Mar 2016 00:35
 Operator : UM/SJ
 Sample : H1625-16 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

35	14.735	2018	2025	2031	rBB2	92111	143601	69.91%	13.558%
36	14.928	2055	2058	2059	rVV	932	797	0.39%	0.075%
37	15.551	2162	2164	2166	rBB	545	522	0.25%	0.049%
38	15.716	2185	2192	2199	rBB2	9223	12845	6.25%	1.213%
39	16.409	2307	2310	2315	rBV3	1059	1269	0.62%	0.120%
40	17.202	2442	2445	2446	rBB3	594	450	0.22%	0.042%
41	17.467	2484	2490	2499	rBB	114531	171965	83.72%	16.236%
42	17.567	2500	2507	2513	rBB2	10172	13333	6.49%	1.259%
43	17.619	2513	2516	2519	rBB2	399	499	0.24%	0.047%
44	17.901	2560	2564	2566	rBV2	455	538	0.26%	0.051%
45	17.990	2577	2579	2584	rVB2	347	398	0.19%	0.038%
46	18.072	2590	2593	2594	rBV	482	433	0.21%	0.041%
47	18.195	2613	2614	2617	rBV	359	402	0.20%	0.038%
48	18.319	2632	2635	2637	rBV	432	640	0.31%	0.060%
49	18.471	2658	2661	2663	rBV	417	474	0.23%	0.045%
50	18.565	2674	2677	2678	rVV	619	485	0.24%	0.046%
51	18.624	2684	2687	2690	rVV	856	723	0.35%	0.068%
52	18.648	2690	2691	2694	rVB	680	449	0.22%	0.042%
53	18.712	2701	2702	2706	rVB2	839	671	0.33%	0.063%
54	18.753	2706	2709	2710	rBV	611	542	0.26%	0.051%
55	18.789	2712	2715	2716	rBV	463	468	0.23%	0.044%
56	18.859	2723	2727	2728	rBV2	610	739	0.36%	0.070%
57	18.877	2728	2730	2733	rVB	540	434	0.21%	0.041%
58	18.918	2735	2737	2740	rBV2	745	549	0.27%	0.052%
59	18.953	2742	2743	2746	rVB2	543	445	0.22%	0.042%
60	18.983	2746	2748	2751	rBV	464	621	0.30%	0.059%
61	19.018	2751	2754	2755	rVB	532	463	0.23%	0.044%
62	19.035	2755	2757	2758	rBV	782	445	0.22%	0.042%
63	19.047	2758	2759	2762	rVB2	1016	712	0.35%	0.067%
64	19.077	2762	2764	2768	rBV3	1392	1798	0.88%	0.170%
65	19.124	2768	2772	2773	rVB3	1043	1009	0.49%	0.095%
66	19.135	2773	2774	2776	rBV3	607	517	0.25%	0.049%
67	19.165	2776	2779	2781	rBV2	831	735	0.36%	0.069%
68	19.206	2785	2786	2790	rVB2	729	662	0.32%	0.063%
69	19.247	2790	2793	2795	rBV2	1115	1090	0.53%	0.103%
70	19.323	2804	2806	2808	rBV3	490	490	0.24%	0.046%
71	19.347	2808	2810	2812	rBV2	956	825	0.40%	0.078%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
 Data File : BG021353.D
 Acq On : 8 Mar 2016 00:35
 Operator : UM/SJ
 Sample : H1625-16 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

72	19.411	2819	2821	2822	rBV	867	859	0.42%	0.081%
73	19.423	2822	2823	2826	rVV3	1236	925	0.45%	0.087%
74	19.453	2826	2828	2830	rVV4	767	799	0.39%	0.075%
75	19.482	2830	2833	2835	rVB3	1753	1770	0.86%	0.167%
76	19.500	2835	2836	2838	rBV2	1282	1046	0.51%	0.099%
77	19.529	2838	2841	2843	rVV3	940	816	0.40%	0.077%
78	19.564	2843	2847	2849	rVB4	886	887	0.43%	0.084%
79	19.617	2854	2856	2858	rBV3	586	636	0.31%	0.060%
80	19.688	2863	2868	2869	rBV5	1487	2055	1.00%	0.194%
81	19.740	2873	2877	2882	rVB3	4112	5191	2.53%	0.490%
82	19.787	2882	2885	2886	rBV3	1319	1225	0.60%	0.116%
83	19.840	2888	2894	2899	rBV	12329	18383	8.95%	1.736%
84	19.887	2899	2902	2907	rVV6	888	1790	0.87%	0.169%
85	19.964	2914	2915	2918	rBV3	1244	1171	0.57%	0.111%
86	20.023	2923	2925	2927	rVB2	1363	1055	0.51%	0.100%
87	20.046	2927	2929	2931	rBV3	838	918	0.45%	0.087%
88	20.093	2936	2937	2938	rBV2	1133	597	0.29%	0.056%
89	20.258	2963	2965	2967	rBV3	1376	1477	0.72%	0.139%
90	20.393	2986	2988	2989	rBV2	1334	798	0.39%	0.075%
91	20.639	3028	3030	3034	rVV5	1960	2048	1.00%	0.193%
92	20.669	3034	3035	3036	rVB	2207	778	0.38%	0.073%
93	21.344	3148	3150	3153	rBV4	3939	5001	2.43%	0.472%
94	21.386	3155	3157	3158	rBV2	2137	1793	0.87%	0.169%
95	21.550	3183	3185	3186	rBV2	2524	1721	0.84%	0.162%
96	21.726	3209	3215	3222	rVB	130950	205397	100.00%	19.393%
97	22.132	3282	3284	3285	rBV2	2238	1731	0.84%	0.163%
98	24.981	3758	3769	3781	rVB2	69337	201251	97.98%	19.001%
99	25.634	3878	3880	3882	rBV2	2031	1568	0.76%	0.148%
100	30.393	4688	4690	4693	rBV4	1736	2218	1.08%	0.209%


Sum of corrected areas: 1059136

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030716\
Data File : BG021353.D
Acq On : 8 Mar 2016 00:35
Operator : UM/SJ
Sample : H1625-16 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
JHFH3

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

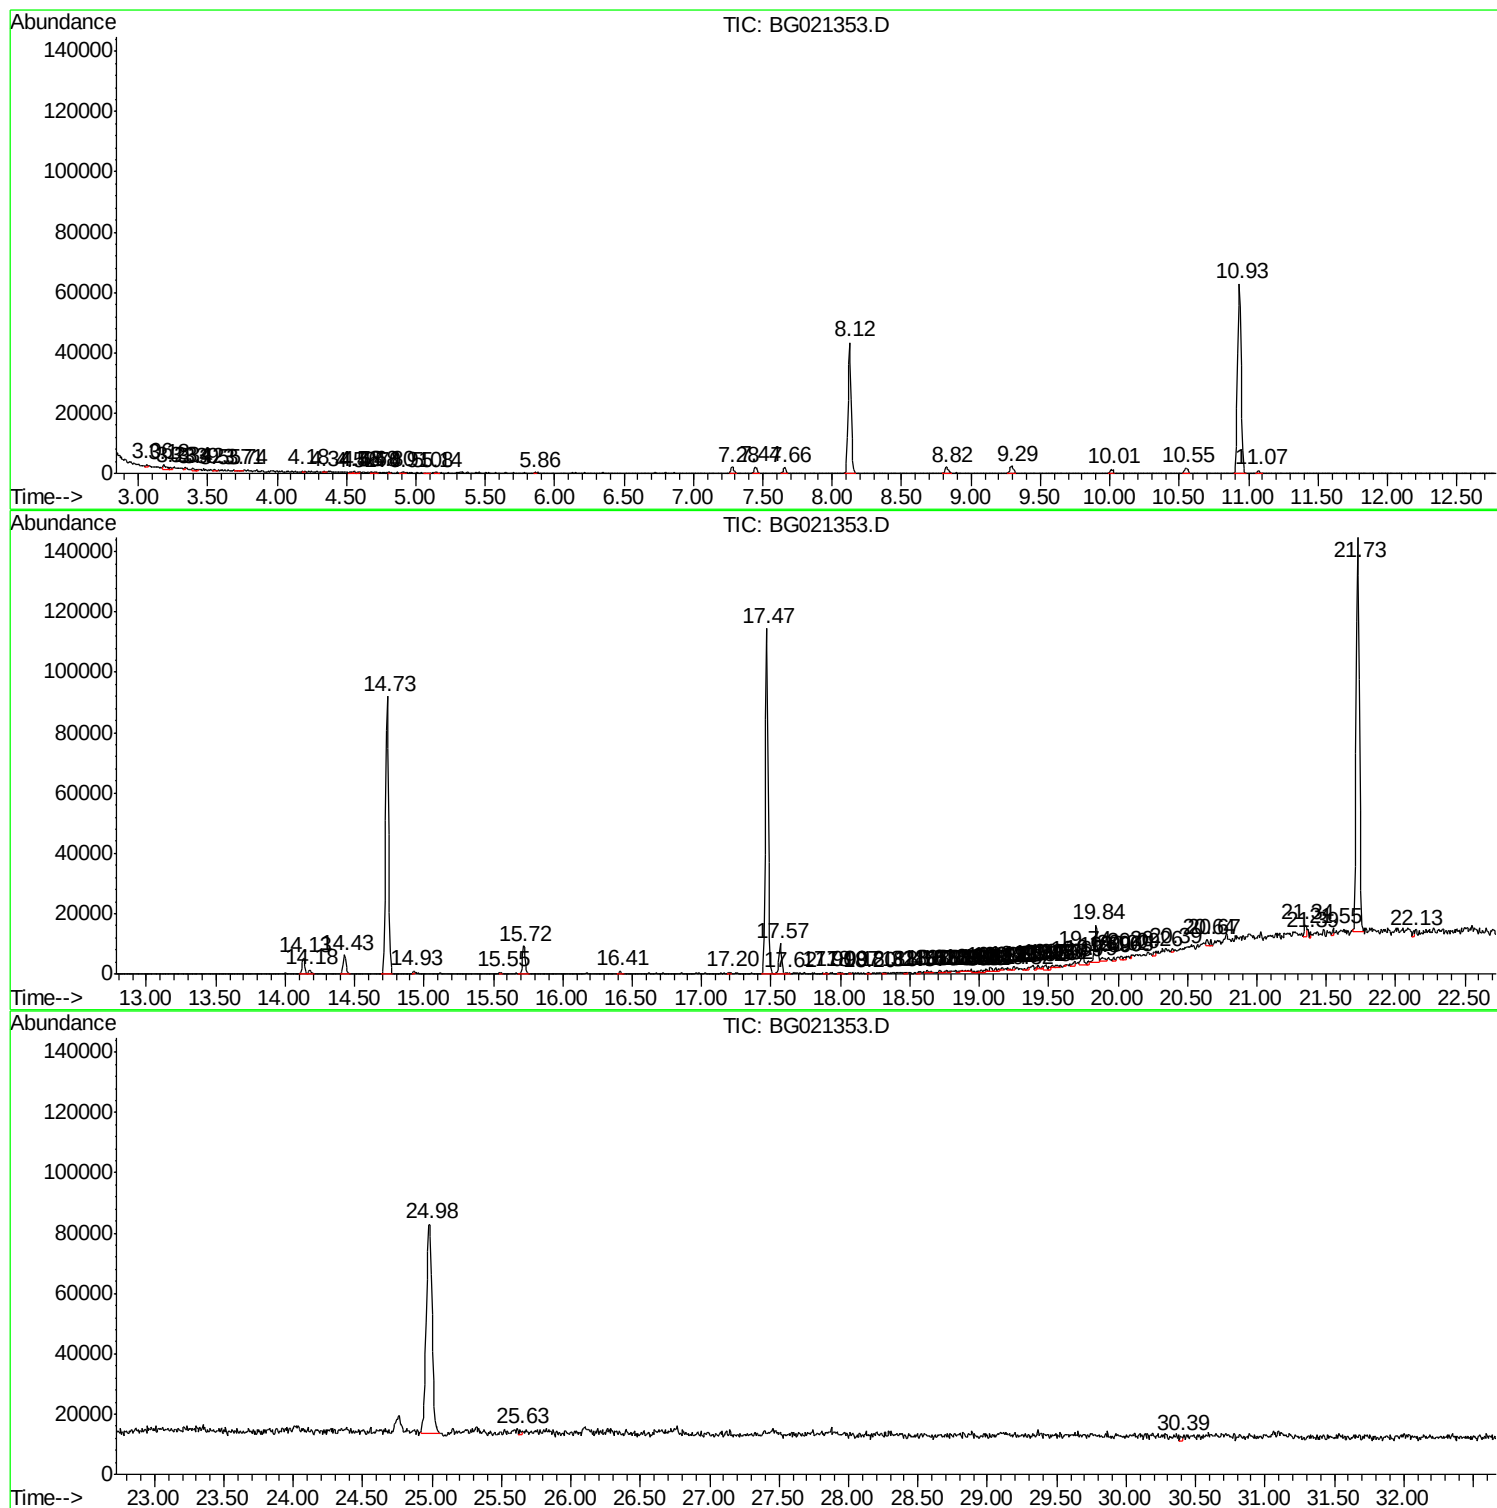

DbaaaPath::ZZ\NRPBMM1BNAAGCDBAA\B00000166\
 DbaaaFile::B0021353DD
 AcqQOn :: 88Mar2006 000355
 Operator::UMMSJ
 Sample::H0025166100X
 Misc ::
 ASSVal::223 SampleMultiplier:11

Instrument :
 BNA_G
 ClientSampleId :
 JHFH3

QcandMebdd::ZZ\NRPBMM1BNAAGCDBAA\B00000166\
 QcandTitle::S00ACALIBRATION

TICLibrary::CC\DATA\B00000166\
 TICIntegratIonParameters:LS6CNTPP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
