

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030717\
 Data File : BG026100.D
 Acq On : 7 Mar 2017 18:13
 Operator : SJ/MA
 Sample : I2095-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BC0

Quant Time: Mar 08 01:02:22 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 07 16:02:09 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	112382	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	475480	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.67	164	274077	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.40	188	650337	20.00	ng/ul	0.00
77) Chrysene-d12	21.64	240	877104	20.00	ng/ul	0.00
85) Perylene-d12	24.82	264	889536	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.50	96	14471	5.54	ng/uL	0.00
5) Phenol-d5	7.22	99	56893	6.81	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	193871	36.76	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	192241	28.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	58239	8.92	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	135038	39.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	129458	45.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	202069	32.04	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	4248	0.49	ng/ul	0.00
43) Dimethylphthalate-d6	14.07	166	813191	45.61	ng/ul	0.00
46) Acenaphthylene-d8	14.36	160	999842	41.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	23180	6.60	ng/ul	0.00
57) Fluorene-d10	15.65	176	739783	42.08	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.76	200	106026	34.75	ng/ul	0.00
70) Anthracene-d10	17.49	188	982049	33.28	ng/ul	0.00
78) Pyrene-d10	19.77	212	1327707	36.80	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.61	264	1505079	38.38	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
20) Nitrobenzene	9.26	77	18161	2.50	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030717\
Data File : BG026100.D
Acq On : 7 Mar 2017 18:13
Operator : SJ/MA
Sample : I2095-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BC0

Quant Time: Mar 08 01:02:22 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 07 16:02:09 2017
Response via : Initial Calibration

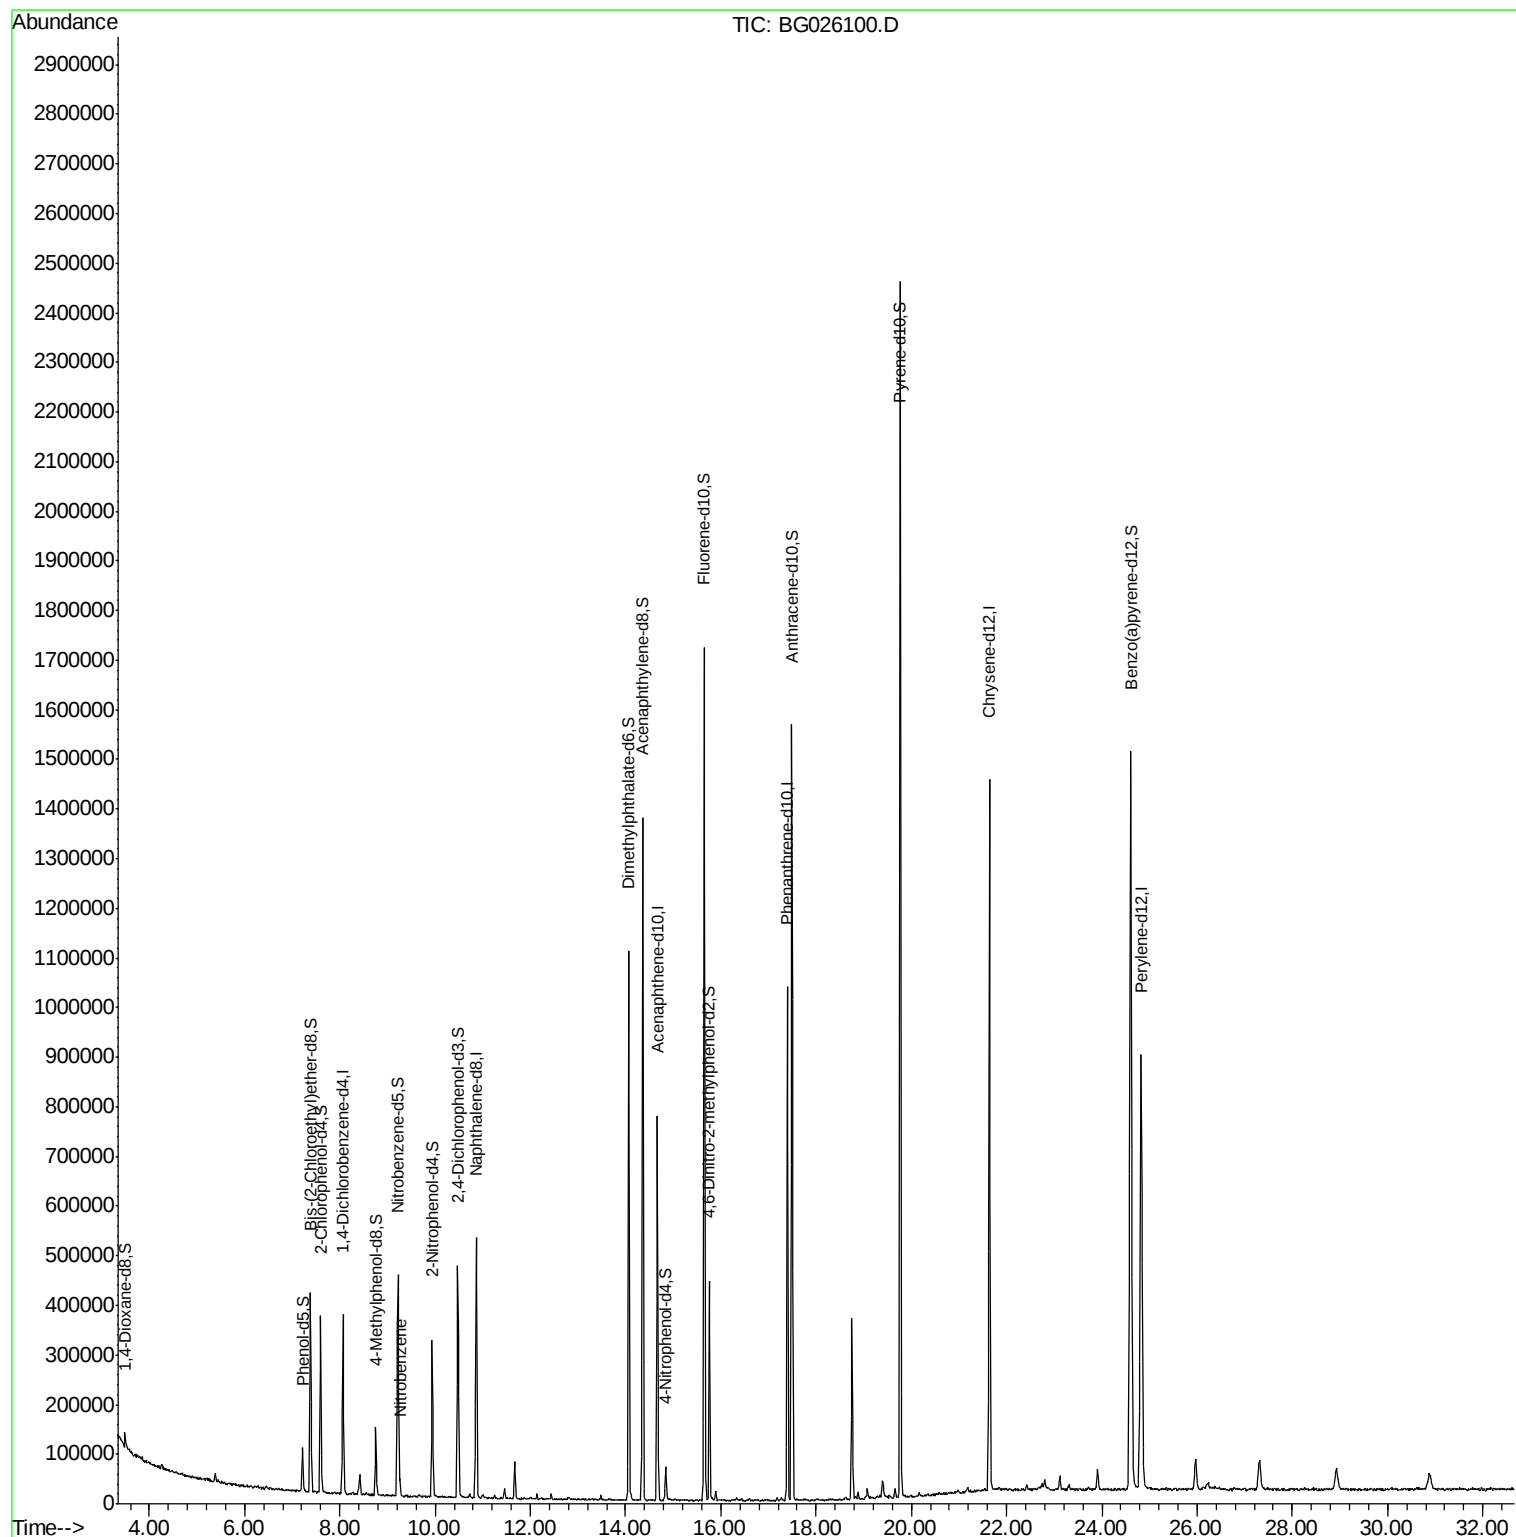

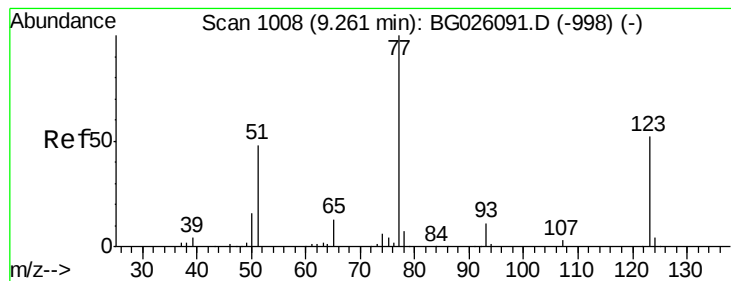

#20
 Nitrobenzene
 Concen: 2.50 ng/ul
 RT: 9.26 min Scan# 1008
 Delta R.T. -0.00 min
 Lab File: BG026100.D
 Acq: 7 Mar 2017 18:13

Instrument :
 BNA_G
 ClientSampleId :
 C0BC0

Tgt Ion: 77 Resp: 18161
 Ion Ratio Lower Upper
 77 100
 123 58.0 39.0 58.4
 65 9.5 10.4 15.6#

