


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030717\
 Data File : BG026104.D
 Acq On : 8 Mar 2017 8:54
 Operator : SJ/MA
 Sample : DFTPP11
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP11

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030717MA.M
 Title : SVOA CALIBRATION
 Last Update : Tue Mar 07 16:02:09 2017

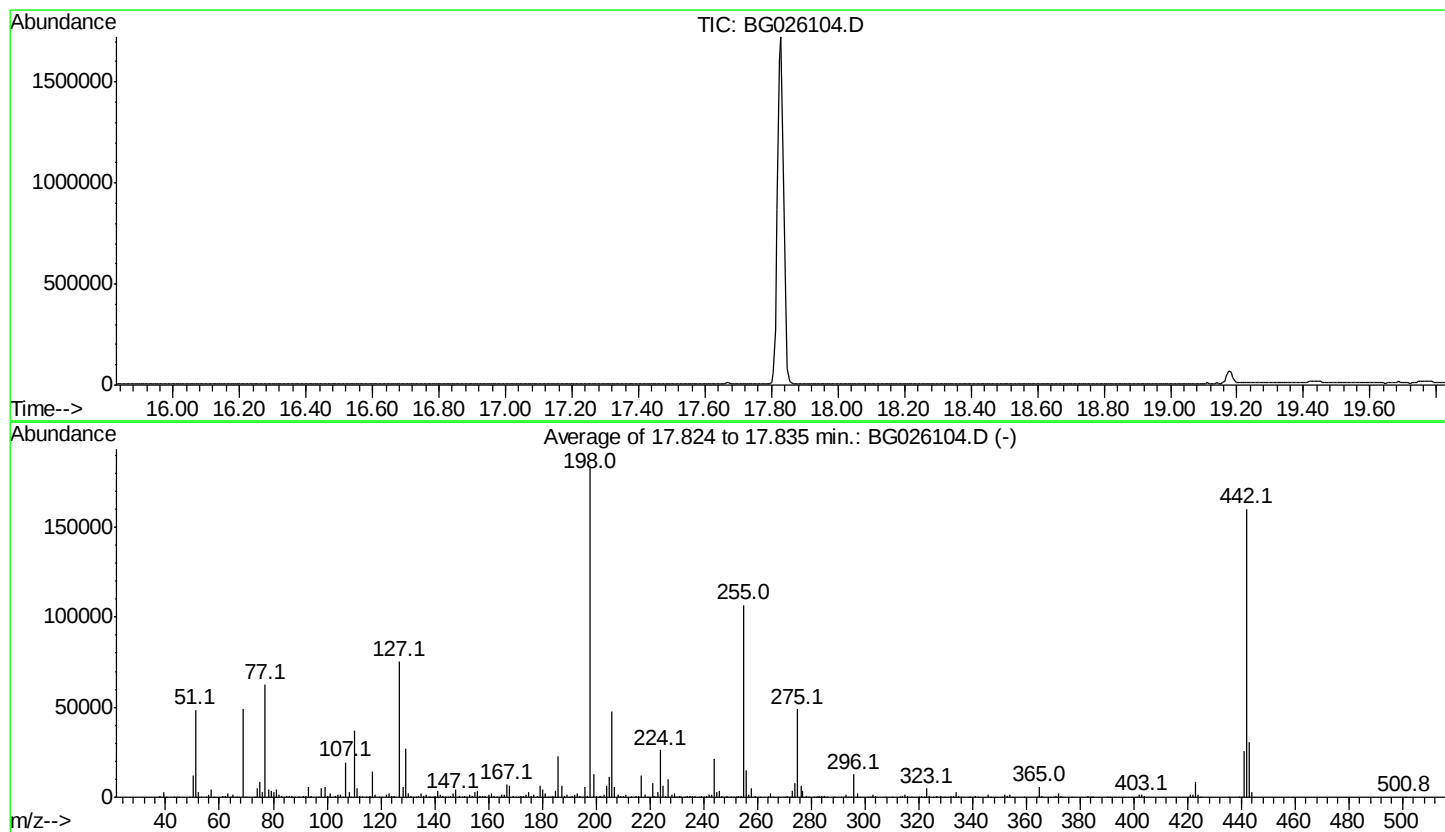

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2459

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.3	48449	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	26.7	49109	PASS
70	69	0.00	2	0.6	303	PASS
127	198	10	80	40.8	75189	PASS
197	198	0.00	2	0.2	412	PASS
198	198	100	100	100.0	184085	PASS
199	198	5	9	7.0	12846	PASS
275	198	10	60	26.5	48712	PASS
365	198	1	100	3.2	5833	PASS
441	442	0.01	100	16.1	25834	PASS
442	198	50	100	86.9	160000	PASS
443	442	15	24	19.0	30365	PASS

Scan 2459 (17.788 min): BG026104.D
DFTPP11

m/z	Abundance
40.10	1364.0
44.10	2886.0
49.10	245.0
51.20	223.0
83.90	289.0
86.00	273.0
139.10	240.0
166.20	162.0
167.10	363.0
207.00	570.0
350.00	163.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

m/z	Abundance
37.20	250.0
38.10	618.0
39.10	3883.0
40.10	1708.0
44.10	3235.0
45.00	299.0
49.00	688.0
50.10	14999.0
51.10	63272.0
52.10	3237.0
53.20	165.0
55.00	486.0
56.00	2146.0
57.10	5278.0
57.90	209.0
61.10	786.0
62.10	719.0
63.10	2278.0
64.10	286.0
65.00	1570.0
67.30	180.0
69.00	60752.0
70.00	523.0
73.10	349.0
74.10	6259.0
75.10	10375.0
76.10	4105.0
77.10	76744.0
78.10	4690.0
79.10	4297.0
80.00	3121.0
81.00	5429.0
82.00	1369.0
83.10	1128.0
84.00	376.0
85.10	774.0
86.00	1557.0
87.00	680.0
88.00	487.0
89.00	170.0
89.70	163.0
91.00	1349.0
92.10	1212.0
93.00	7453.0
94.00	571.0
96.10	349.0
98.00	5594.0
99.10	6421.0
100.00	645.0
101.00	2852.0
103.10	823.0
104.00	1725.0
105.00	1618.0
107.10	25024.0
108.10	3154.0
110.10	44488.0
111.00	6483.0
112.00	977.0
112.90	217.0
116.00	1177.0
117.10	16840.0
118.00	1213.0
119.10	271.0
119.90	189.0
122.00	1852.0
123.00	2337.0
124.00	1258.0
125.00	929.0
127.10	88576.0
128.10	6879.0
129.10	31608.0
130.00	2647.0
131.10	600.0
132.20	297.0
133.00	181.0
134.00	890.0
135.00	2771.0
136.10	1075.0
137.10	1982.0
137.80	491.0
139.00	279.0
140.00	447.0
141.00	3973.0
142.00	1436.0
143.10	1079.0
143.90	163.0
145.00	279.0
146.10	857.0
147.10	2458.0
148.00	5288.0
149.00	1223.0
150.10	344.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

151.10	427.0
151.80	331.0
153.00	1367.0
154.10	1047.0
155.10	3217.0
156.10	4133.0
157.10	891.0
158.00	638.0
158.90	817.0
160.00	1110.0
161.10	2294.0
162.00	657.0
164.10	269.0
165.00	1767.0
166.10	1564.0
167.10	8347.0
168.10	7139.0
169.00	1024.0
170.20	349.0
171.00	285.0
172.00	919.0
173.00	1222.0
174.10	1383.0
175.10	3714.0
175.90	573.0
177.10	1688.0
178.10	921.0
179.00	7164.0
180.00	4619.0
181.10	2769.0
182.00	437.0
184.10	601.0
185.10	3841.0
186.10	26656.0
187.10	8416.0
188.10	843.0
189.00	1455.0
190.00	213.0
191.00	643.0
192.00	1865.0
193.00	2299.0
194.10	957.0
195.00	259.0
196.10	6050.0
198.00	203072.0
199.00	14066.0
200.00	1116.0
201.00	500.0
201.50	1125.0
203.00	1483.0
204.10	7356.0
205.10	12984.0
206.10	54432.0
207.10	6769.0
208.10	1338.0
209.00	584.0
210.10	835.0
211.00	2023.0
213.00	286.0
214.90	491.0
216.00	966.0
217.00	12740.0
218.10	1449.0
221.10	9278.0
221.80	1840.0
223.10	3264.0
224.10	29368.0
225.10	6988.0
226.10	1201.0
227.00	9860.0
228.00	1356.0
229.00	2047.0
229.90	181.0
231.10	825.0
233.00	236.0
234.10	605.0
235.00	590.0
236.10	463.0
237.00	1137.0
238.10	161.0
239.10	353.0
240.00	539.0
241.00	994.0
242.10	1569.0
243.10	1888.0
244.10	24312.0
245.00	3520.0
246.00	3936.0
247.00	560.0
248.00	219.0
248.90	737.0
250.30	326.0
250.90	413.0
252.00	300.0
253.10	778.0
255.00	113784.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

256.10	17416.0
257.00	1195.0
258.00	5551.0
259.00	864.0
260.00	197.0
261.00	158.0
264.20	244.0
265.00	2223.0
265.90	419.0
268.00	152.0
270.10	321.0
271.00	477.0
272.10	528.0
273.00	3716.0
274.10	8025.0
275.10	52832.0
276.10	7023.0
277.00	3504.0
278.00	550.0
279.00	169.0
282.00	261.0
283.10	446.0
284.00	615.0
285.10	621.0
286.00	189.0
288.10	241.0
288.90	181.0
291.10	203.0
292.10	250.0
293.10	1193.0
294.20	266.0
295.10	278.0
296.00	13008.0
297.10	1674.0
301.00	151.0
302.00	255.0
303.00	1304.0
304.10	483.0
308.00	194.0
310.00	231.0
312.90	235.0
314.10	679.0
315.00	1335.0
316.00	913.0
317.10	193.0
321.00	543.0
323.10	5434.0
324.00	820.0
325.20	246.0
326.90	569.0
328.10	487.0
332.00	520.0
333.10	568.0
334.10	2918.0
335.10	416.0
341.10	650.0
342.10	236.0
345.90	1129.0
351.10	153.0
352.10	1158.0
353.10	1002.0
354.10	1390.0
355.10	207.0
359.10	179.0
365.00	5193.0
366.00	787.0
371.00	331.0
372.00	2067.0
373.10	535.0
383.10	765.0
384.40	180.0
390.00	347.0
401.00	210.0
402.00	841.0
403.10	1121.0
404.10	496.0
421.10	749.0
422.10	1122.0
423.10	6926.0
424.10	1389.0
425.00	250.0
441.10	20936.0
442.10	138432.0
443.10	27576.0
444.10	2432.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

m/z	Abundance
37.20	161.0
38.10	729.0
39.10	3173.0
40.00	1599.0
43.10	170.0
44.10	2492.0
45.10	157.0
49.10	589.0
50.10	14650.0
51.10	55352.0
52.10	3471.0
53.00	223.0
55.10	315.0
56.10	1701.0
57.10	4485.0
58.00	168.0
61.10	751.0
62.10	1033.0
63.10	3005.0
64.10	564.0
65.10	1677.0
66.20	154.0
69.00	55976.0
69.90	213.0
73.00	290.0
74.10	6342.0
75.10	9909.0
76.10	3366.0
77.10	69976.0
78.10	5054.0
79.10	4381.0
80.00	2914.0
81.10	4597.0
82.10	1381.0
83.10	1063.0
83.90	277.0
85.00	778.0
86.00	1382.0
87.00	696.0
88.00	267.0
89.10	253.0
91.00	1089.0
92.10	1282.0
93.10	5651.0
94.10	492.0
96.00	475.0
97.00	188.0
98.00	5765.0
99.10	6356.0
100.10	467.0
101.00	3027.0
103.00	1037.0
104.10	2222.0
105.00	1233.0
106.10	563.0
107.10	20176.0
108.10	3345.0
110.00	42752.0
111.00	5854.0
112.00	913.0
113.10	323.0
114.60	170.0
116.00	1140.0
117.00	16240.0
118.00	1572.0
120.00	497.0
122.10	1007.0
123.10	2144.0
124.00	812.0
125.10	1286.0
127.10	89344.0
128.10	6591.0
129.00	32272.0
130.10	2929.0
131.10	797.0
132.00	356.0
133.00	370.0
134.10	1158.0
135.10	2756.0
136.00	1211.0
137.00	2036.0
138.10	465.0
139.40	170.0
140.00	408.0
141.00	4072.0
142.10	1885.0
143.10	914.0
144.10	390.0
145.00	180.0
146.10	645.0
147.10	2502.0
148.10	4443.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

149.10	1175.0
150.00	503.0
150.90	544.0
152.00	322.0
153.00	1541.0
154.10	1201.0
155.10	3217.0
156.10	3786.0
157.00	727.0
158.00	750.0
159.00	432.0
160.00	1568.0
161.00	2041.0
162.00	506.0
164.00	439.0
165.00	1801.0
166.00	1881.0
167.00	8434.0
168.10	7296.0
169.10	827.0
170.00	211.0
171.10	220.0
172.00	670.0
173.00	930.0
174.10	1710.0
175.10	3314.0
176.00	701.0
177.00	2005.0
178.10	849.0
179.00	7113.0
180.00	4375.0
181.10	1812.0
182.00	392.0
183.10	299.0
184.10	536.0
185.10	3596.0
186.10	27336.0
187.10	7088.0
188.10	600.0
189.00	1954.0
190.00	369.0
191.10	816.0
192.10	2257.0
193.00	2730.0
194.00	584.0
196.00	6493.0
198.00	216000.0
199.00	15513.0
200.10	1465.0
201.60	1235.0
202.10	394.0
203.00	1264.0
204.10	7095.0
205.10	13077.0
206.10	54960.0
207.10	7058.0
208.10	1527.0
209.00	820.0
210.00	826.0
211.10	2080.0
213.20	259.0
215.00	686.0
216.00	1354.0
217.00	14371.0
218.00	1902.0
221.00	9321.0
223.10	3856.0
224.10	31000.0
225.10	7790.0
226.10	1188.0
227.00	12083.0
228.10	1582.0
229.00	2378.0
230.10	385.0
231.10	1065.0
231.80	205.0
233.10	221.0
234.00	1071.0
235.00	910.0
236.10	587.0
237.10	851.0
238.10	234.0
239.00	675.0
240.00	331.0
240.90	803.0
242.00	1357.0
243.10	1643.0
244.10	23696.0
245.10	3553.0
246.00	4674.0
247.00	918.0
248.00	330.0
248.90	896.0
250.00	440.0
251.00	294.0
251.90	248.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

252.20	267.0
253.20	612.0
254.00	1502.0
255.00	127800.0
256.00	17296.0
257.10	1765.0
258.00	5937.0
259.10	922.0
261.10	361.0
264.10	289.0
265.00	2363.0
266.00	473.0
271.00	617.0
273.00	3865.0
274.10	9960.0
275.10	56144.0
276.10	7924.0
277.00	3944.0
278.10	785.0
279.00	309.0
283.00	598.0
284.10	374.0
285.10	800.0
286.10	217.0
289.00	327.0
291.20	182.0
292.00	224.0
293.00	1127.0
294.10	441.0
296.10	13839.0
297.00	2327.0
298.00	222.0
301.10	322.0
302.00	573.0
303.10	1491.0
304.00	667.0
307.90	259.0
310.10	278.0
313.10	234.0
314.10	515.0
315.00	1722.0
316.10	1218.0
317.00	187.0
320.10	185.0
321.00	430.0
322.00	344.0
323.10	5959.0
324.10	944.0
326.90	1141.0
328.00	532.0
329.80	162.0
332.10	529.0
333.10	351.0
334.10	3305.0
335.10	862.0
339.10	157.0
341.10	631.0
346.00	1272.0
346.90	297.0
351.00	165.0
352.10	1534.0
353.10	1238.0
354.10	1469.0
355.00	330.0
364.00	174.0
365.00	7239.0
366.10	859.0
370.00	159.0
371.10	496.0
372.10	2849.0
373.10	750.0
376.90	177.0
383.10	958.0
384.00	308.0
390.10	358.0
391.00	170.0
402.10	1459.0
403.10	1301.0
404.10	487.0
421.10	1517.0
422.10	1655.0
423.10	10644.0
424.10	1916.0
425.10	162.0
435.50	159.0
439.20	243.0
441.10	33304.0
442.10	197632.0
443.10	36568.0
444.10	4022.0
500.80	166.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

m/z	Abundance
38.10	227.0
39.10	2133.0
40.00	1608.0
44.10	3240.0
45.20	245.0
49.00	526.0
50.10	7647.0
51.10	27392.0
52.10	1229.0
56.00	1275.0
57.10	2374.0
61.00	343.0
62.10	513.0
63.10	1685.0
64.00	153.0
65.10	837.0
69.00	30600.0
70.00	173.0
73.00	250.0
74.10	2754.0
75.10	5085.0
76.10	2064.0
77.10	40736.0
78.10	2788.0
79.10	2665.0
80.10	1766.0
81.00	2670.0
82.00	651.0
83.00	1009.0
83.80	190.0
85.00	540.0
86.00	594.0
87.00	575.0
87.90	302.0
91.00	608.0
92.00	580.0
93.00	3388.0
94.10	193.0
96.10	303.0
98.10	3036.0
99.10	3531.0
100.00	325.0
101.10	1586.0
103.00	601.0
104.10	1168.0
105.10	878.0
107.10	12735.0
108.10	1720.0
109.00	638.0
110.00	22712.0
111.00	3698.0
112.00	369.0
113.00	162.0
116.00	812.0
117.10	9549.0
118.10	927.0
120.10	315.0
122.10	563.0
123.00	1435.0
124.10	503.0
125.10	546.0
127.10	47648.0
128.10	3739.0
129.00	17536.0
130.00	1506.0
131.00	498.0
132.00	153.0
132.80	198.0
134.10	547.0
135.10	1407.0
136.10	747.0
137.10	1367.0
139.00	220.0
140.00	318.0
141.00	2343.0
142.10	709.0
143.00	705.0
145.00	188.0
146.00	351.0
147.10	1100.0
148.00	3269.0
149.10	738.0
150.00	223.0
151.10	345.0
151.90	380.0
153.00	918.0
154.10	488.0
155.10	1598.0
156.10	2433.0
157.00	401.0
158.00	486.0
159.00	367.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

160.10	852.0
161.00	1522.0
161.90	385.0
163.00	183.0
165.00	964.0
166.10	733.0
167.10	5079.0
168.00	4959.0
169.00	640.0
170.20	222.0
171.00	375.0
171.90	316.0
172.90	533.0
174.00	1410.0
175.10	2466.0
176.00	466.0
177.00	864.0
178.20	466.0
179.00	4758.0
180.10	3013.0
181.10	1588.0
182.00	243.0
183.20	170.0
184.00	504.0
185.00	2326.0
186.10	14890.0
187.10	4209.0
188.10	646.0
189.00	971.0
190.10	257.0
191.00	555.0
192.00	1111.0
193.00	1780.0
194.00	420.0
195.10	252.0
196.10	3842.0
196.90	1236.0
198.00	133184.0
199.00	8961.0
200.00	450.0
201.50	519.0
202.00	364.0
203.00	795.0
204.10	3908.0
205.10	7852.0
206.10	32840.0
207.10	4207.0
208.10	869.0
208.90	448.0
210.10	480.0
211.10	1276.0
215.10	324.0
216.10	656.0
217.00	8495.0
218.00	1245.0
219.10	214.0
221.00	5687.0
222.00	1072.0
223.00	1853.0
224.10	17640.0
225.10	4743.0
226.00	416.0
227.00	7529.0
228.00	912.0
229.00	1346.0
230.00	233.0
231.00	545.0
234.00	347.0
235.10	582.0
236.00	373.0
237.00	603.0
238.00	312.0
238.90	167.0
240.00	160.0
241.00	412.0
242.00	1150.0
243.00	1191.0
244.10	16424.0
245.00	2291.0
246.10	2242.0
247.10	639.0
247.90	239.0
249.00	652.0
250.10	405.0
250.90	297.0
252.00	364.0
253.20	460.0
255.00	78968.0
256.00	11124.0
257.10	737.0
258.00	4334.0
259.00	825.0
263.90	152.0
265.00	1680.0
270.90	374.0
272.10	294.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11

273.00	2388.0
274.00	5644.0
275.10	37160.0
276.00	4493.0
277.00	3120.0
278.00	521.0
281.00	177.0
282.20	230.0
283.00	631.0
284.00	277.0
285.00	424.0
292.00	246.0
293.00	1003.0
294.00	320.0
295.00	393.0
296.00	10931.0
297.10	1456.0
302.00	181.0
303.10	1293.0
304.00	233.0
310.10	158.0
313.10	202.0
314.00	424.0
315.00	1097.0
316.10	658.0
317.10	231.0
321.10	380.0
322.20	303.0
323.10	3343.0
324.10	626.0
327.00	687.0
328.00	578.0
332.10	279.0
333.00	253.0
334.10	2167.0
335.10	488.0
336.00	189.0
338.60	182.0
341.00	404.0
346.00	1061.0
347.00	178.0
352.00	899.0
353.10	833.0
354.10	1275.0
355.00	286.0
365.00	5069.0
366.00	971.0
371.20	422.0
372.10	1771.0
373.10	529.0
383.10	662.0
384.00	215.0
385.10	174.0
389.90	235.0
391.00	252.0
402.10	1017.0
403.10	1420.0
404.10	403.0
421.10	1194.0
422.10	1051.0
423.10	7209.0
424.10	1176.0
425.00	343.0
439.90	308.0
441.10	23264.0
442.10	143936.0
443.10	26952.0
444.10	2480.0

Instrument :
BNA_G
ClientSampleId :
DFTPP11