
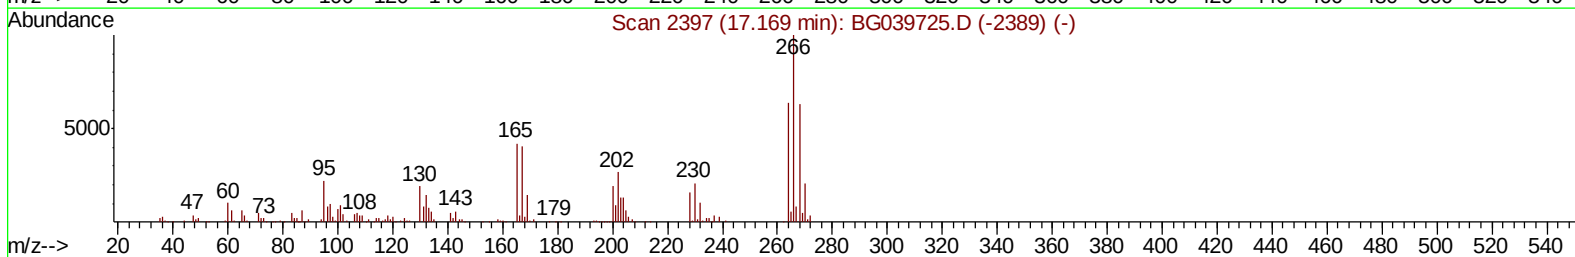
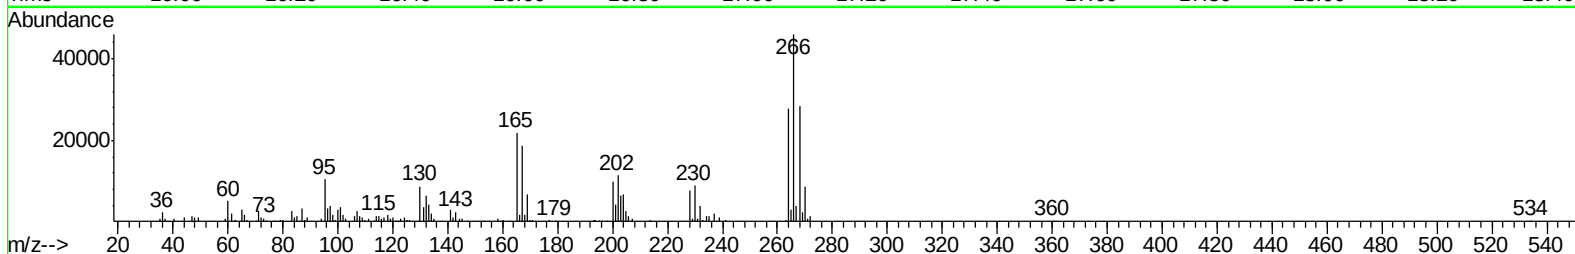


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030719\
 Data File : BG039800.D
 Acq On : 7 Mar 2019 13:35
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 08 04:32:14 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030419.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 04 14:38:15 2019
 Response via : Initial Calibration

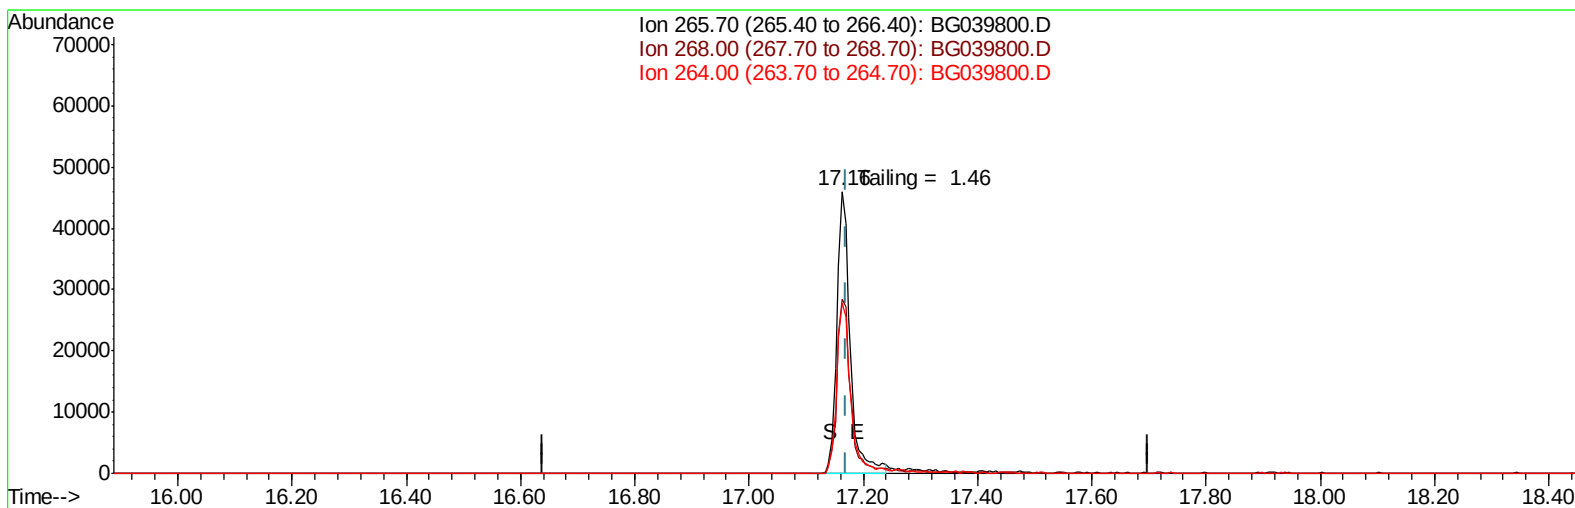

TIC: BG039800.D

(70) Pentachlorophenol (C)

17.163min (-0.007) 29168.60ng

response 72671

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.90
264.00	65.10	60.49
0.00	0.00	0.00