
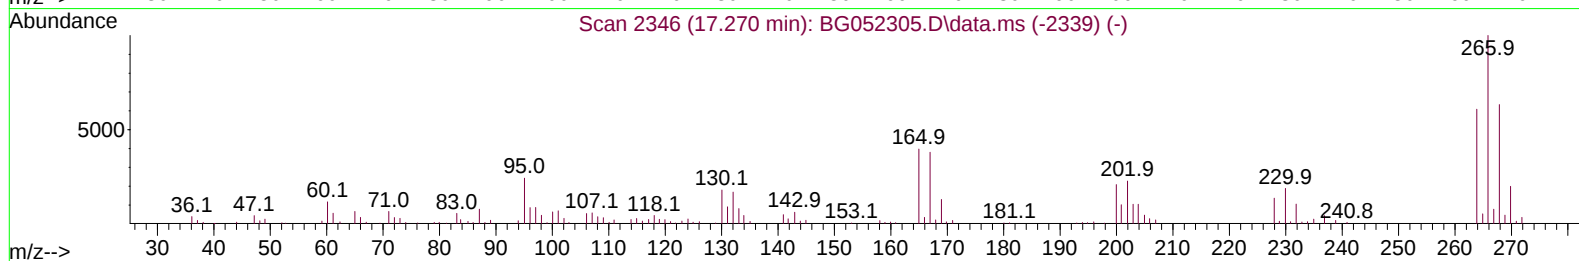
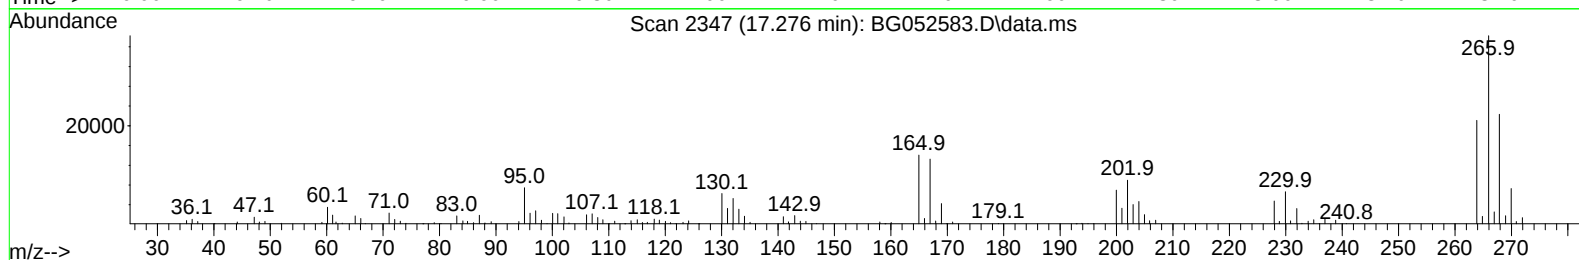


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030722\  
Data File : BG052583.D  
Acq On    : 7 Mar 2022    9:22  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Mar 07 11:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 07 11:25:10 2022
Response via : Initial Calibration

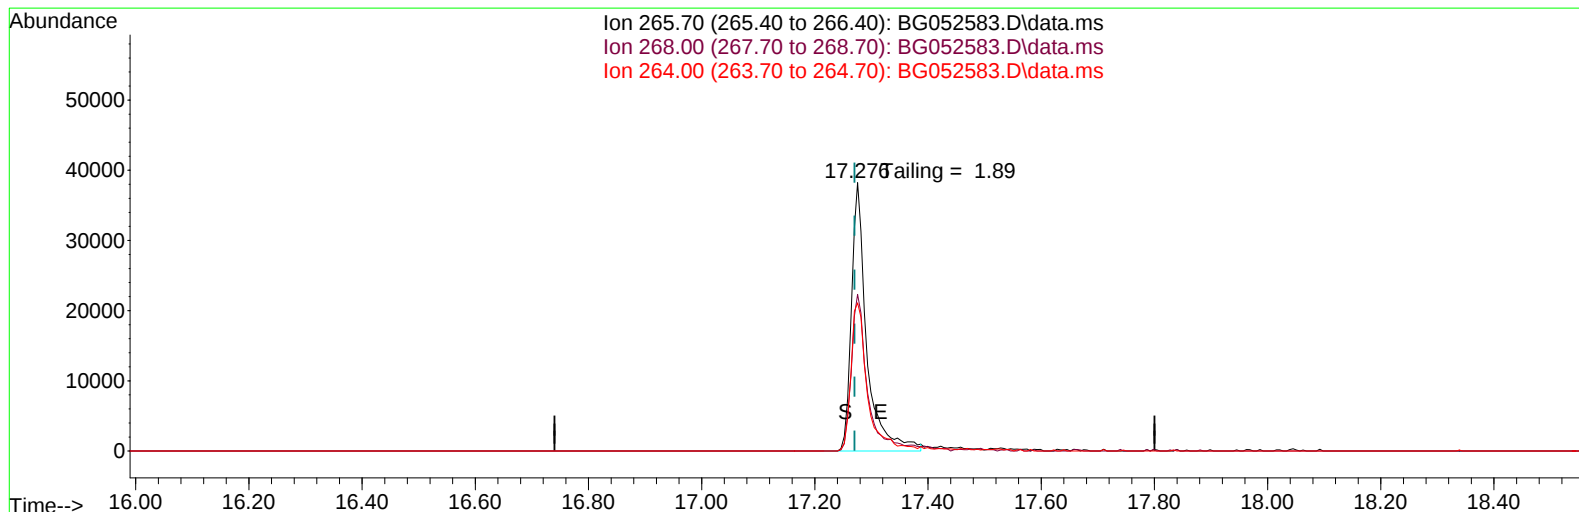

TIC: BG052583.D\data.ms

(70) Pentachlorophenol (C)




17.276min (+ 0.006) 75256.91 ng

response 72843

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	58.37
264.00	65.20	55.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030722\
Data File : BG052583.D
Acq On : 7 Mar 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 11:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 07 11:25:10 2022
Response via : Initial Calibration

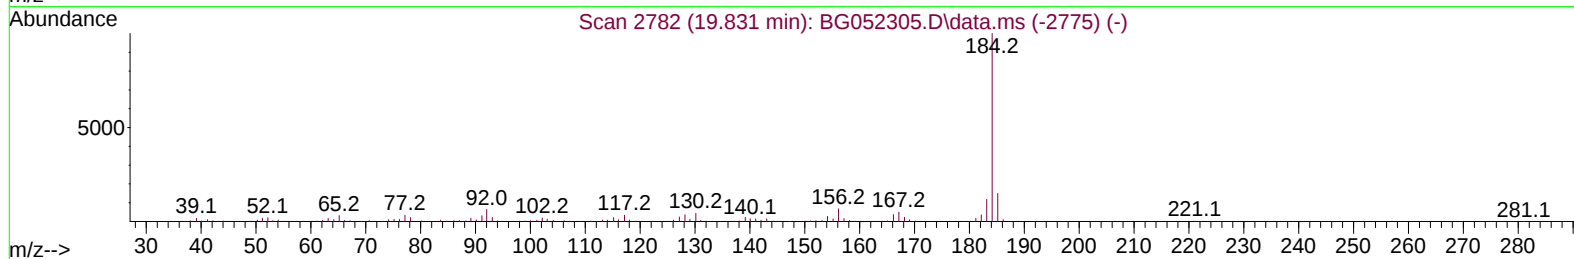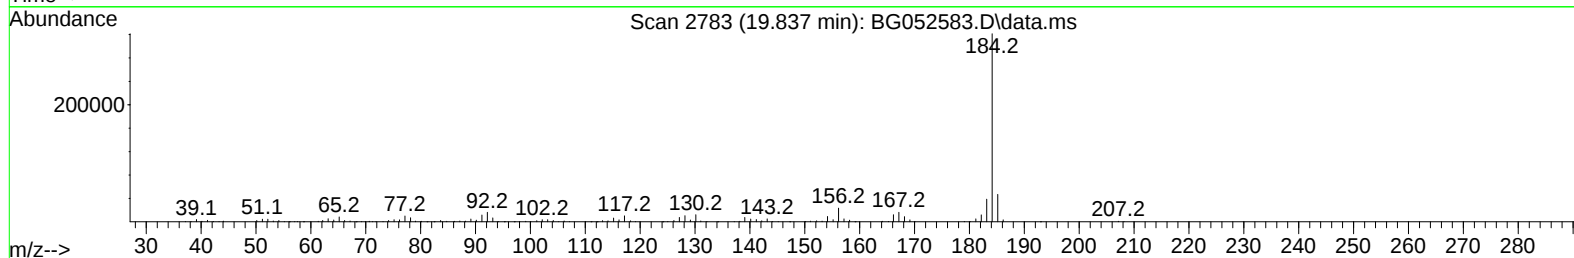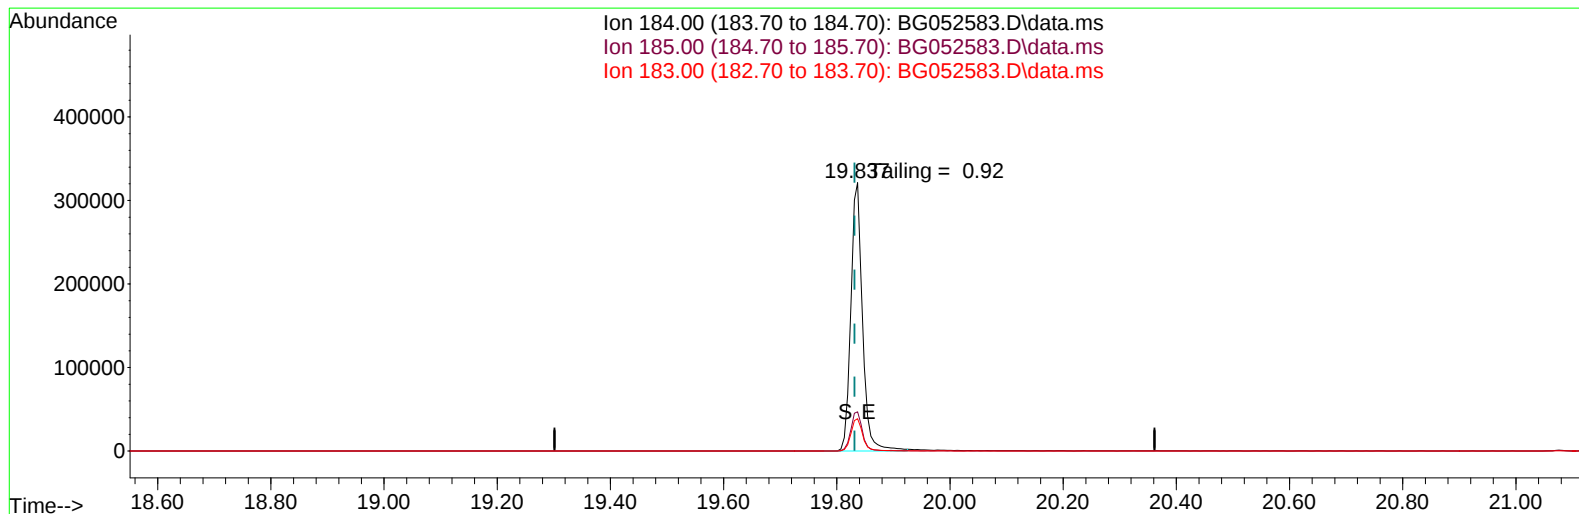

TIC: BG052583.D\data.ms

(77) Benzidine**19.837min (+ 0.006) 44930.32 ng****response 463709**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.64
183.00	12.20	12.07
0.00	0.00	0.00