
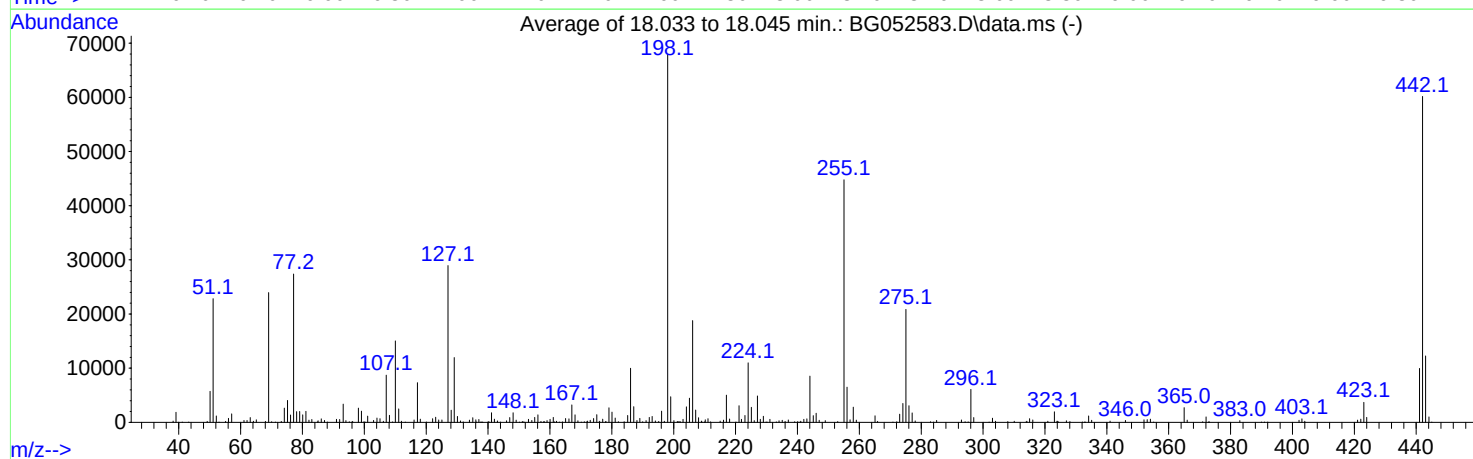


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030722\
 Data File : BG052583.D
 Acq On : 7 Mar 2022 9:22
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 08 01:09:10 2022

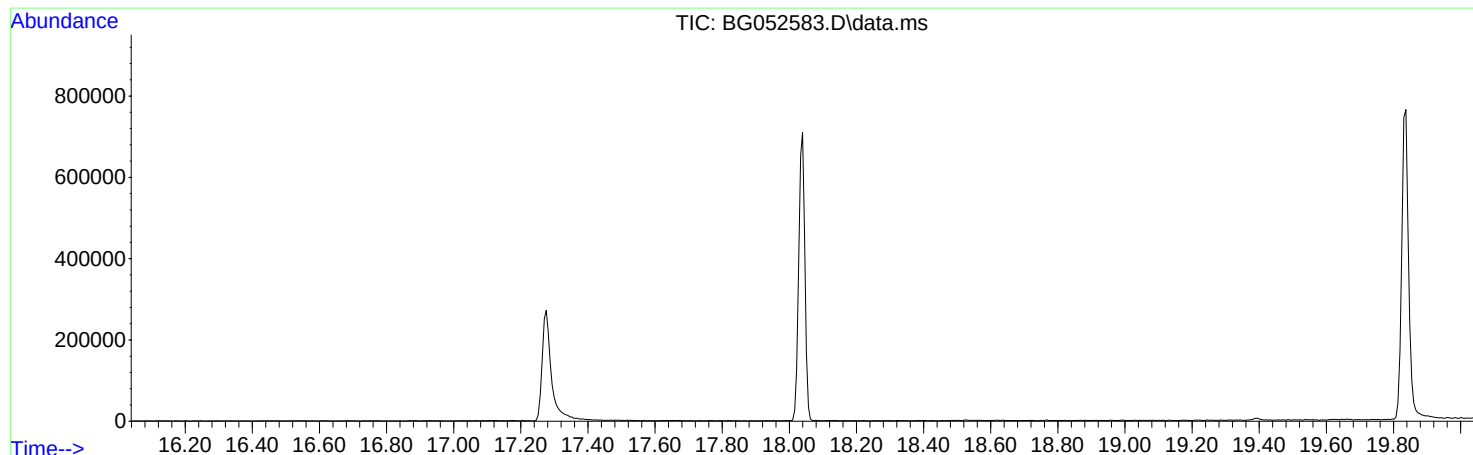




AutoFind: Scans 2476, 2477, 2478; Background Corrected with Scan 2469

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.6	22843	PASS
68	69	0.00	2	0.8	192	PASS
69	198	0.00	100	35.3	23966	PASS
70	69	0.00	2	0.5	126	PASS
127	198	10	80	42.6	28960	PASS
197	198	0.00	2	0.3	215	PASS
198	198	100	100	100.0	67915	PASS
199	198	5	9	7.0	4728	PASS
275	198	10	60	30.7	20869	PASS
365	198	1	100	4.0	2706	PASS
441	198	0.01	100	14.7	9952	PASS
442	442	50	100	100.0	60163	PASS
443	442	15	24	20.4	12272	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030722\
Data File : BG052583.D
Acq On : 7 Mar 2022 9:22
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 07 11:29:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 07 11:25:10 2022
Response via : Initial Calibration

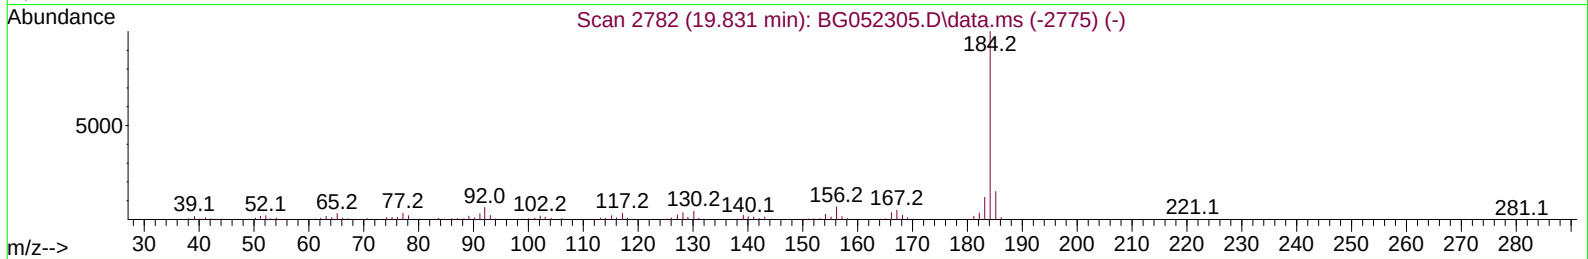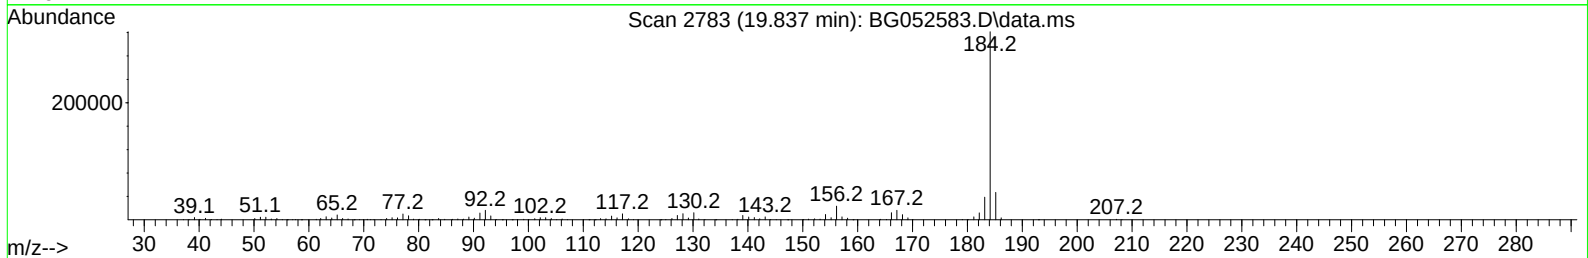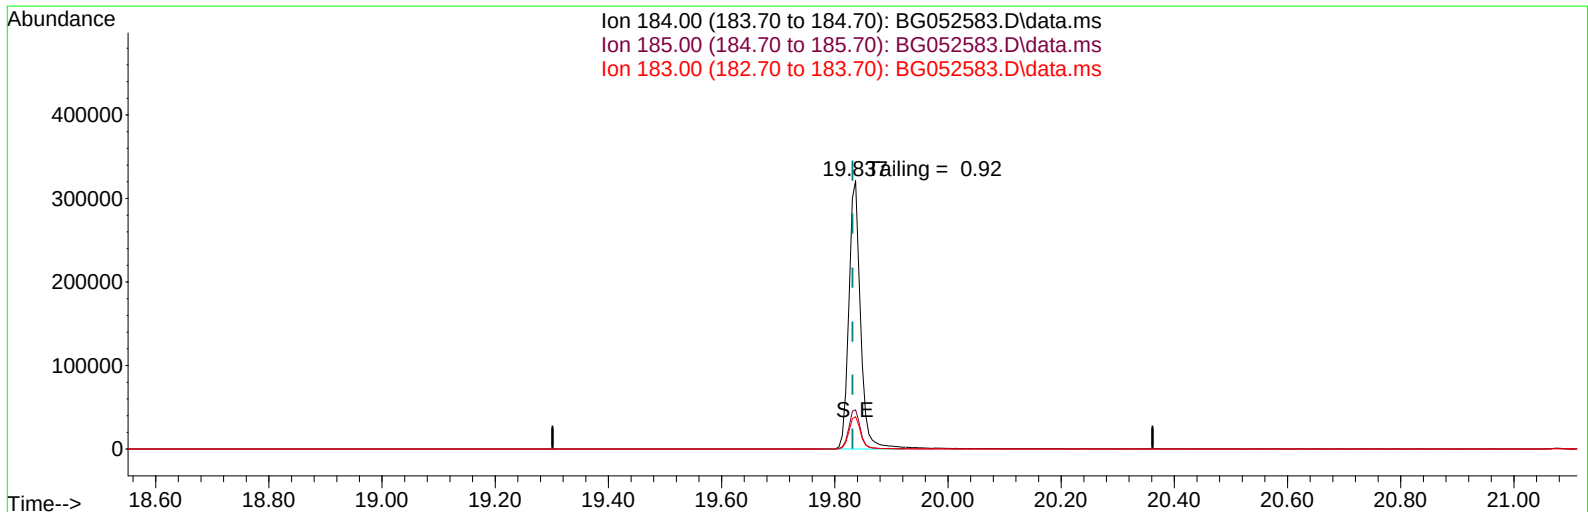

TIC: BG052583.D\data.ms

(77) Benzidine

19.837min (+ 0.006) 44930.32 ng

response 463709

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.64
183.00	12.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2022	BNA_G	<u>BG052583.D</u>
Compound Name	Response	Retention Time
DDT	249525	21.07
DDD	1881	20.62
DDE	62	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1943	251468	0.77

Instrument :
BNA_G
ClientSampleId :
DFTPP