




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030723\  
 Data File : BG056872.D  
 Acq On : 7 Mar 2023 15:19  
 Operator : CG/JU  
 Sample : SSTD16079  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SSTD160426

Manual IntegrationsAPPROVED

Quant Time: Mar 07 16:00:33 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG030723.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Mar 07 15:23:28 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/08/2023  
 Supervised By :Jagrut Upadhyay 03/08/2023

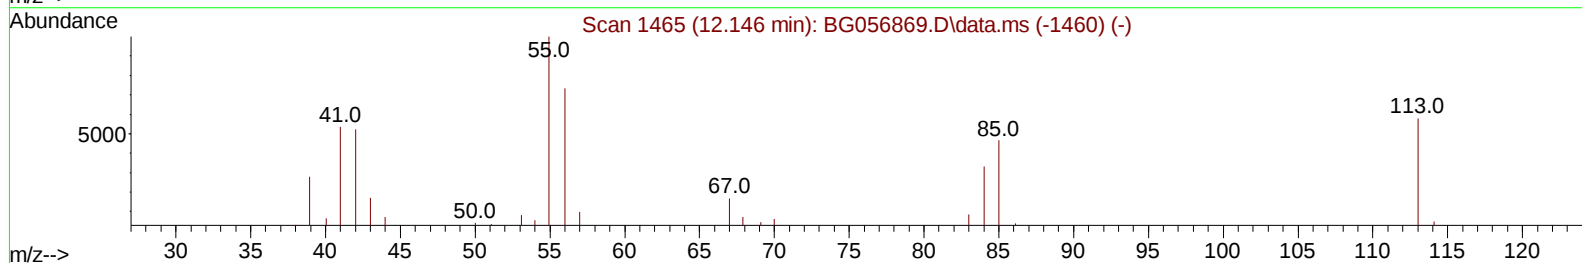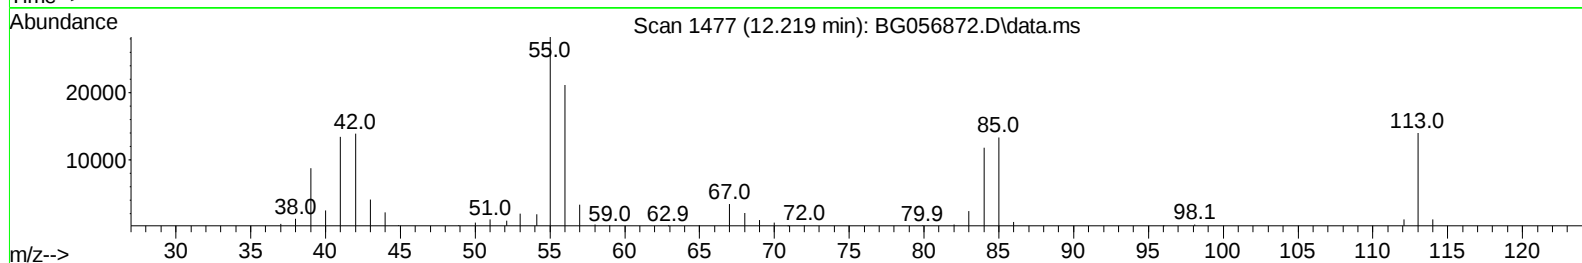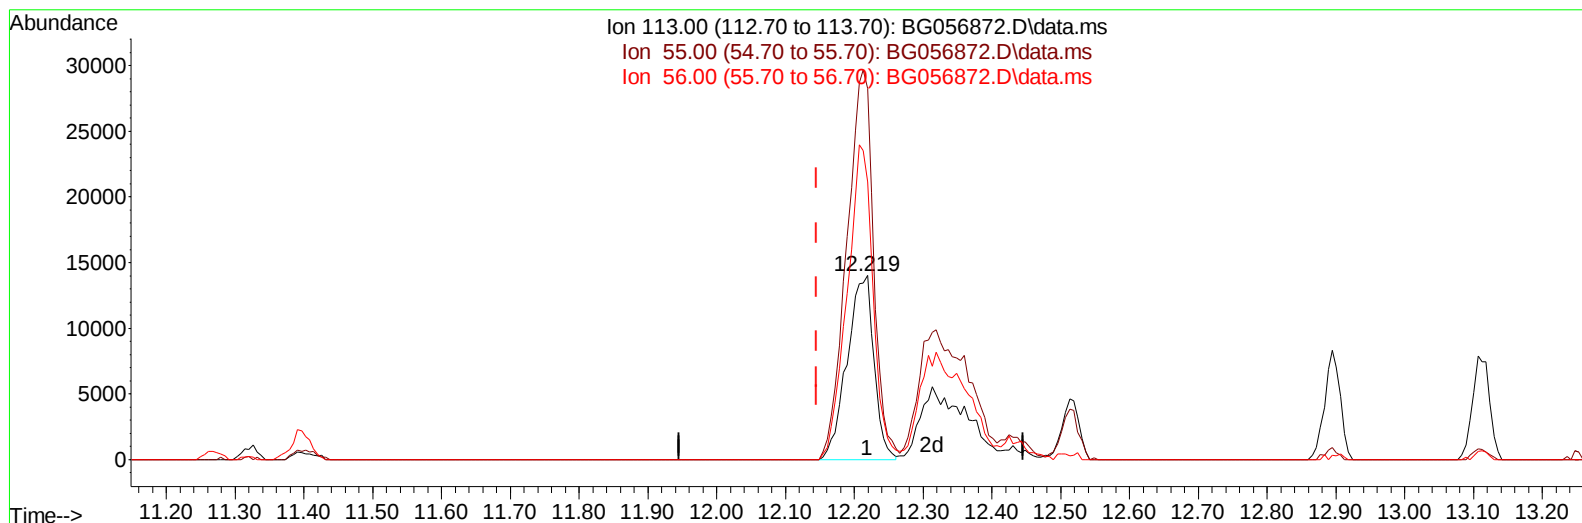

TIC: BG056872.D\data.ms

**(34) Caprolactam**

12.219min (+ 0.073) 79.48 ng/ul

response 38025

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100.00 | 100.00 |
| 55.00  | 188.50 | 201.53 |
| 56.00  | 137.50 | 150.77 |
| 0.00   | 0.00   | 0.00   |




Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030723\  
 Data File : BG056872.D  
 Acq On : 7 Mar 2023 15:19  
 Operator : CG/JU  
 Sample : SSTD16079  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SSTD160426

Manual IntegrationsAPPROVED

Quant Time: Mar 07 16:00:33 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG030723.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Mar 07 15:23:28 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/08/2023  
 Supervised By :Jagrut Upadhyay 03/08/2023

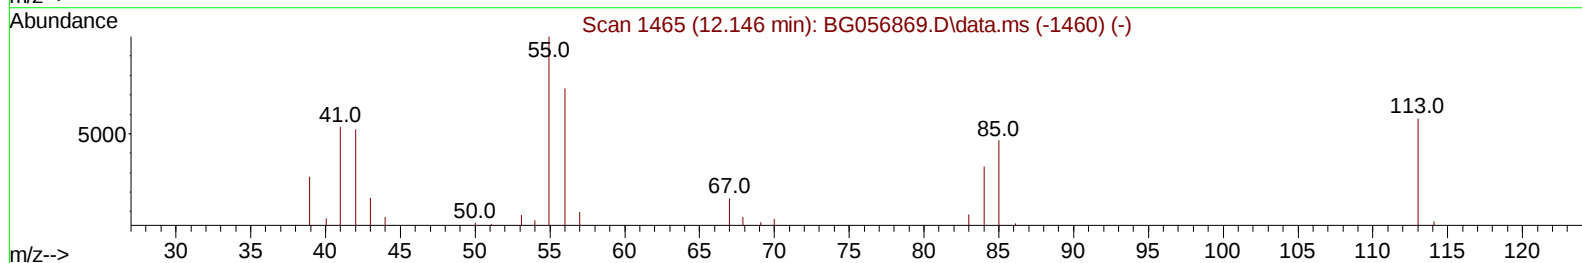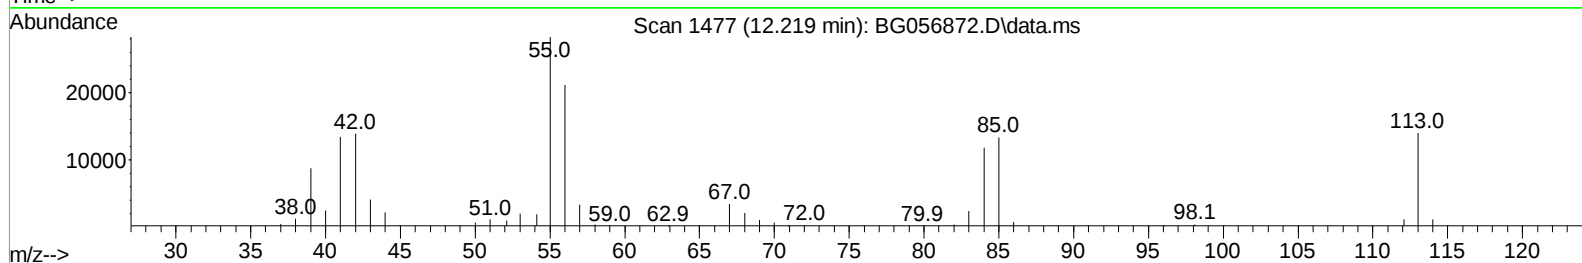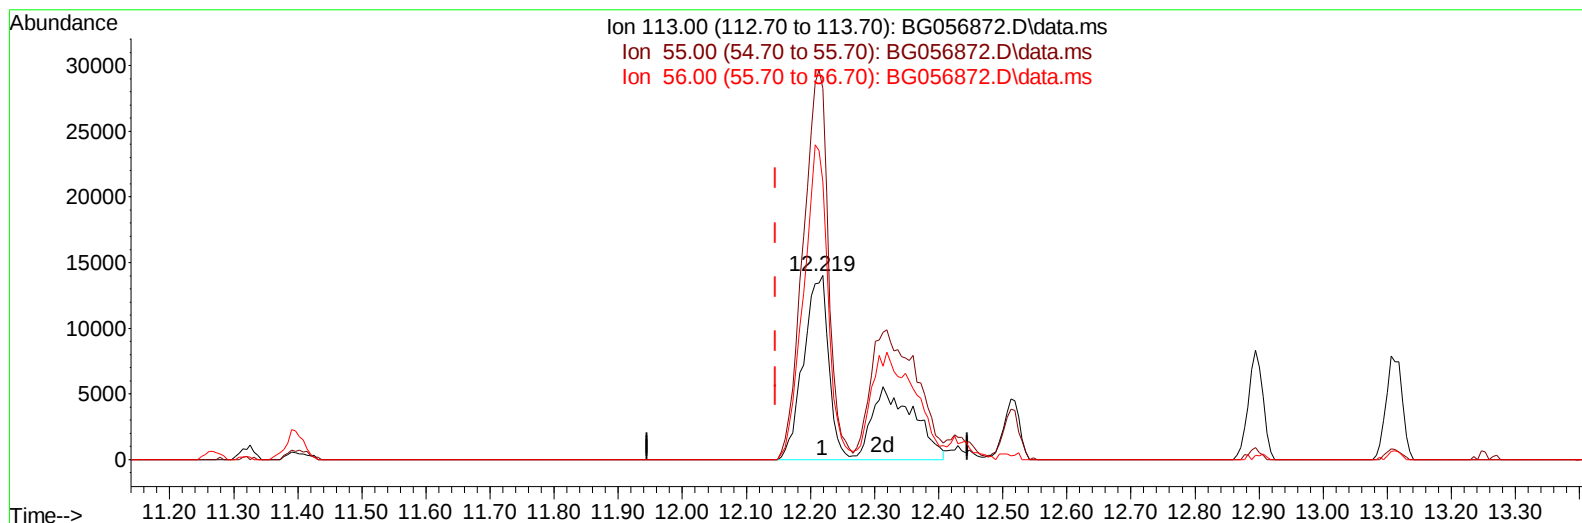

TIC: BG056872.D\data.ms

**(34) Caprolactam**

12.219min (+ 0.073) 131.38 ng/u1 m

response 62854

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 113.00 | 100.00 | 100.00 |
| 55.00  | 188.50 | 201.53 |
| 56.00  | 137.50 | 150.77 |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030723\  
 Data File : BG056872.D  
 Acq On : 7 Mar 2023 15:19  
 Operator : CG/JU  
 Sample : SSTD16079  
 Misc :  
 ALS Vial : 8 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 SSTD160426

Manual IntegrationsAPPROVED

Quant Time: Mar 07 16:00:33 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG030723.M  
 Quant Title : SVOA CALIBRATION  
 QLast Update : Tue Mar 07 15:23:28 2023  
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/08/2023  
 Supervised By :Jagrut Upadhyay 03/08/2023

| Compound                      | R.T.   | QIon | Response | Conc    | Units  | Dev(Min) |
|-------------------------------|--------|------|----------|---------|--------|----------|
| -----                         |        |      |          |         |        |          |
| Internal Standards            |        |      |          |         |        |          |
| 1) 1,4-Dichlorobenzene-d4     | 8.423  | 152  | 15135    | 20.000  | ng/ul  | 0.00     |
| 20) Naphthalene-d8            | 11.267 | 136  | 68596    | 20.000  | ng/ul  | 0.00     |
| 38) Acenaphthene-d10          | 15.039 | 164  | 52190    | 20.000  | ng/ul  | 0.00     |
| 64) Phenanthrene-d10          | 17.783 | 188  | 127077   | 20.000  | ng/ul  | 0.00     |
| 79) Chrysene-d12              | 22.119 | 240  | 120694   | 20.000  | ng/ul  | 0.00     |
| 88) Perylene-d12              | 25.674 | 264  | 132147   | 20.000  | ng/ul  | 0.00     |
| System Monitoring Compounds   |        |      |          |         |        |          |
| 3) 1,4-Dioxane-d8             | 0.000  | 96   | 0d       | 0.000   | ng/uL  |          |
| 4) Pyridine-d5                | 4.128  | 84   | 209553   | 162.732 | ng/ul  | 0.00     |
| 7) Phenol-d5                  | 7.554  | 99   | 264982   | 173.758 | ng/ul  | 0.01     |
| 9) Bis-(2-Chloroethyl)eth...  | 7.730  | 67   | 153450   | 156.874 | ng/ul  | 0.00     |
| 11) 2-Chlorophenol-d4         | 0.000  | 132  | 0d       | 0.000   | ng/ul  |          |
| 15) 4-Methylphenol-d8         | 9.128  | 113  | 193592   | 166.800 | ng/ul  | 0.02     |
| 21) Nitrobenzene-d5           | 0.000  | 128  | 0d       | 0.000   | ng/ul  |          |
| 24) 2-Nitrophenol-d4          | 0.000  | 143  | 0d       | 0.000   | ng/ul  |          |
| 28) 2,4-Dichlorophenol-d3     | 0.000  | 165  | 0d       | 0.000   | ng/ul  |          |
| 31) 4-Chloroaniline-d4        | 11.396 | 131  | 262335   | 150.990 | ng/ul  | 0.00     |
| 46) Dimethylphthalate-d6      | 0.000  | 166  | 0d       | 0.000   | ng/ul  |          |
| 49) Acenaphthylene-d8         | 0.000  | 160  | 0d       | 0.000   | ng/ul  |          |
| 54) 4-Nitrophenol-d4          | 15.227 | 143  | 111740   | 144.936 | ng/ul  | 0.03     |
| 60) Fluorene-d10              | 0.000  | 176  | 0d       | 0.000   | ng/ul  |          |
| 65) 4,6-Dinitro-2-methylph... | 16.144 | 200  | 146634   | 159.578 | ng/ul  | 0.02     |
| 73) Anthracene-d10            | 0.000  | 188  | 0d       | 0.000   | ng/ul  |          |
| 81) Pyrene-d10                | 0.000  | 212  | 0d       | 0.000   | ng/ul  |          |
| 92) Benzo(a)pyrene-d12        | 0.000  | 264  | 0d       | 0.000   | ng/ul  |          |
| Target Compounds              |        |      |          |         |        |          |
|                               |        |      |          |         |        | Qvalue   |
| 5) Pyridine                   | 4.152  | 79   | 221693   | 163.435 | ng/ul  | 99       |
| 6) Benzaldehyde               | 7.542  | 77   | 83882    | 94.294  | ng/ul  | 94       |
| 8) Phenol                     | 7.583  | 94   | 268128   | 172.105 | ng/ul  | 94       |
| 10) Bis(2-Chloroethyl)ether   | 7.824  | 93   | 179920   | 162.436 | ng/ul  | 99       |
| 13) 2-Methylphenol            | 8.852  | 108  | 196086   | 170.955 | ng/ul  | 91       |
| 14) 2,2'-oxybis(1-Chloropr... | 8.946  | 45   | 241870   | 158.039 | ng/ul  | 95       |
| 16) Acetophenone              | 9.264  | 105  | 321264   | 160.478 | ng/ul  | 95       |
| 18) 4-Methylphenol            | 9.205  | 108  | 207497   | 165.560 | ng/ul  | 90       |
| 32) 4-Chloroaniline           | 11.426 | 127  | 256314   | 150.473 | ng/ul  | 96       |
| 34) Caprolactam               | 12.219 | 113  | 62854m   | 131.383 | ng/ul  |          |
| 40) Hexachlorocyclopentadiene | 13.230 | 237  | 228034   | 177.753 | ng/ul  | 95       |
| 51) 3-Nitroaniline            | 14.945 | 138  | 110477   | 129.842 | ng/ul  | 96       |
| 53) 2,4-Dinitrophenol         | 15.145 | 184  | 110255   | 167.240 | ng/ul  | 95       |
| 55) 4-Nitrophenol             | 15.245 | 109  | 142864   | 143.497 | ng/ul  | 99       |
| 63) 4-Nitroaniline            | 16.114 | 138  | 109097   | 129.132 | ng/ul  | 91       |
| 66) 4,6-Dinitro-2-methylph... | 16.161 | 198  | 140980   | 160.495 | ng/ul# | 93       |
| 70) Atrazine                  | 17.219 | 200  | 225893   | 144.344 | ng/ul  | 98       |
| 71) Pentachlorophenol         | 17.425 | 266  | 170031   | 171.031 | ng/ul  | 98       |
| 77) Carbazole                 | 18.183 | 167  | 880836   | 146.466 | ng/ul  | 100      |
| 84) 3,3'-Dichlorobenzidine    | 21.990 | 252  | 381864   | 124.872 | ng/ul  | 99       |
| 89) Di-n-octyl phthalate      | 23.277 | 149  | 1104785  | 151.968 | ng/ul  | 100      |
| -----                         |        |      |          |         |        |          |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030723\  
Data File : BG056872.D  
Acq On : 7 Mar 2023 15:19  
Operator : CG/JU  
Sample : SSTD16079  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
SSTD160426

**Manual IntegrationsAPPROVED**

Reviewed By :Christian Giraldo 03/08/2023  
Supervised By :Jagrut Upadhyay 03/08/2023

Quant Time: Mar 07 16:00:33 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG030723.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Mar 07 15:23:28 2023  
Response via : Initial Calibration

| Compound                                                                   | R.T. | Q | Ion | Response | Conc | Units | Dev(Min) |
|----------------------------------------------------------------------------|------|---|-----|----------|------|-------|----------|
| -----                                                                      |      |   |     |          |      |       |          |
| (#) = qualifier out of range (m) = manual integration (+) = signals summed |      |   |     |          |      |       |          |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG030723\  
Data File : BG056872.D  
Acq On : 7 Mar 2023 15:19  
Operator : CG/JU  
Sample : SSTD16079  
Misc :  
ALS Vial : 8 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
SSTD160426

## Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/08/2023  
Supervised By :Jagrut Upadhyay 03/08/2023

Quant Time: Mar 07 16:00:33 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\SFAM-EPA-BG030723.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Mar 07 15:23:28 2023  
Response via : Initial Calibration

