


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030724\
Data File : BG060583.D
Acq On : 7 Mar 2024 10:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030724.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 08 03:35:45 2024

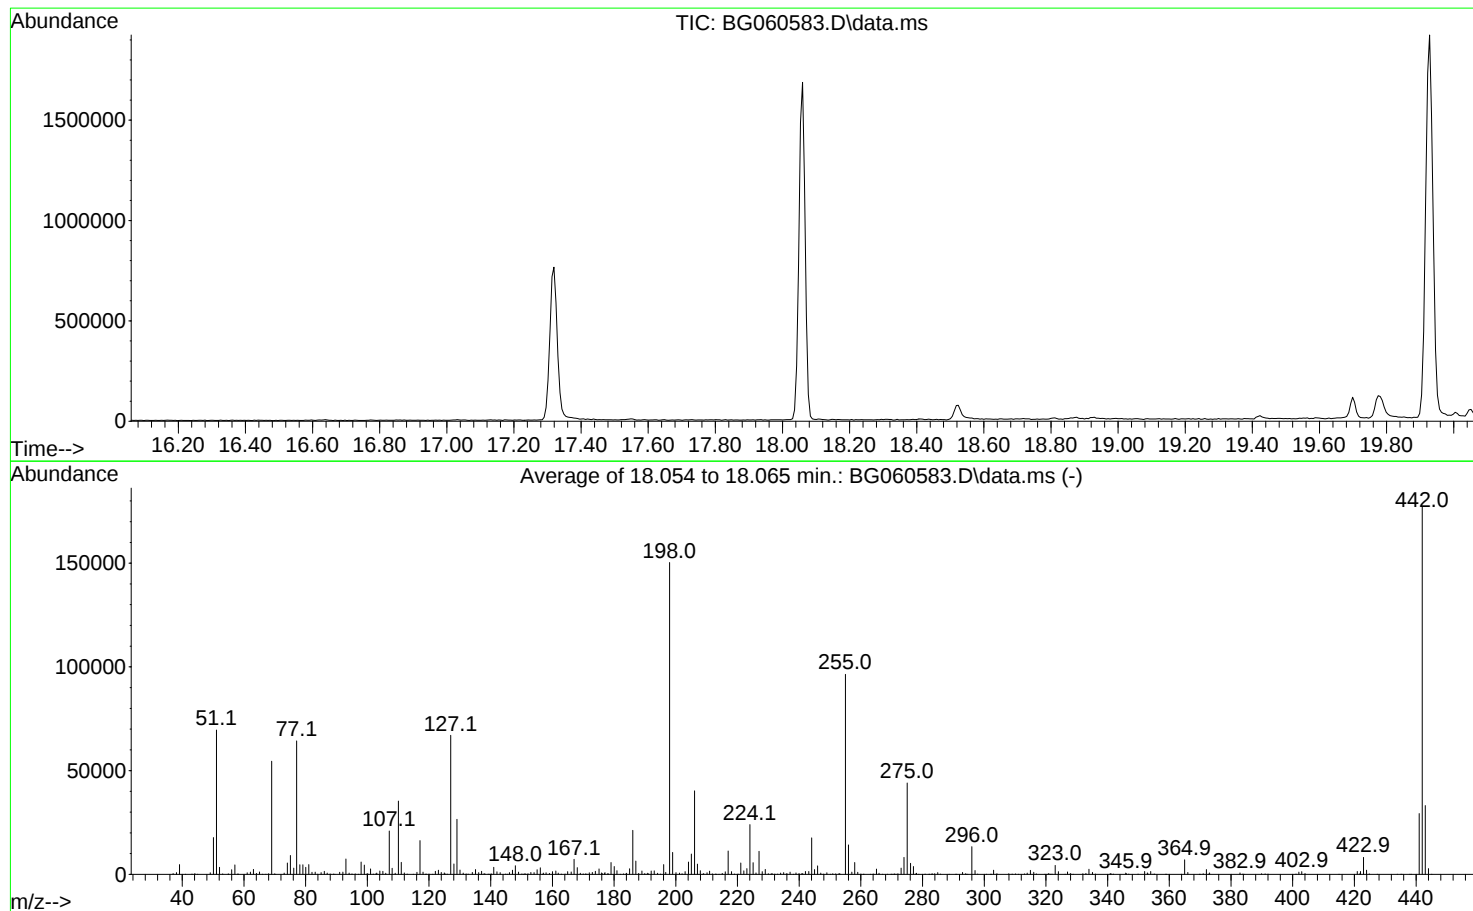




AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	69579	PASS
68	69	0.00	2	0.6	325	PASS
69	198	0.00	100	36.3	54509	PASS
70	69	0.00	2	0.5	273	PASS
127	198	10	80	44.6	66992	PASS
197	198	0.00	2	0.6	905	PASS
198	198	100	100	100.0	150304	PASS
199	198	5	9	7.0	10573	PASS
275	198	10	60	29.3	44032	PASS
365	198	1	100	4.7	6999	PASS
441	198	0.01	100	19.5	29299	PASS
442	442	50	100	100.0	177323	PASS
443	442	15	24	18.7	33155	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030724\
Data File : BG060583.D
Acq On : 7 Mar 2024 10:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 08 03:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 03:35:45 2024
Response via : Initial Calibration

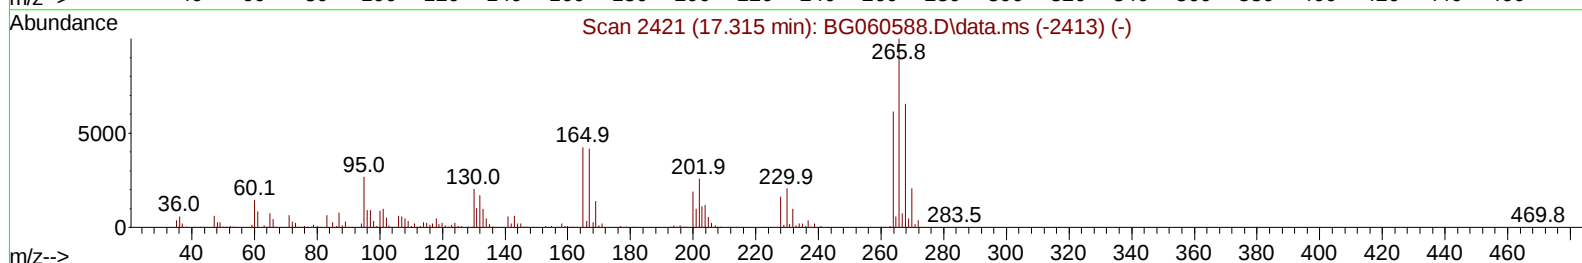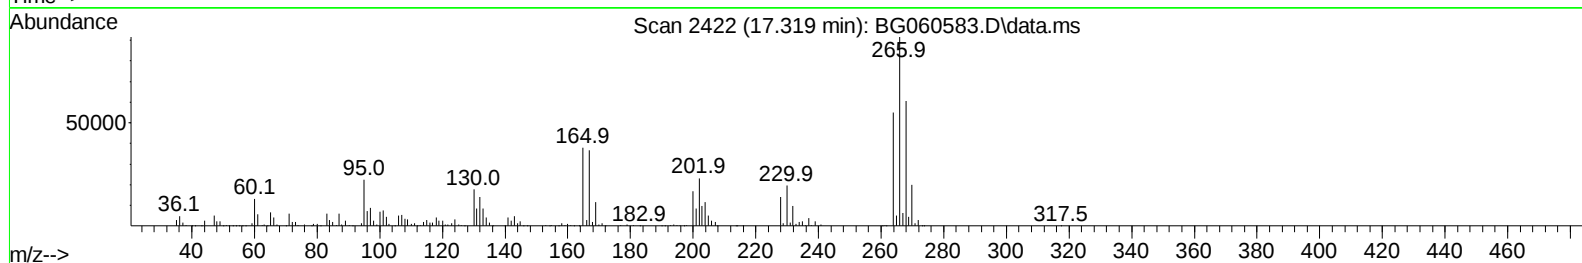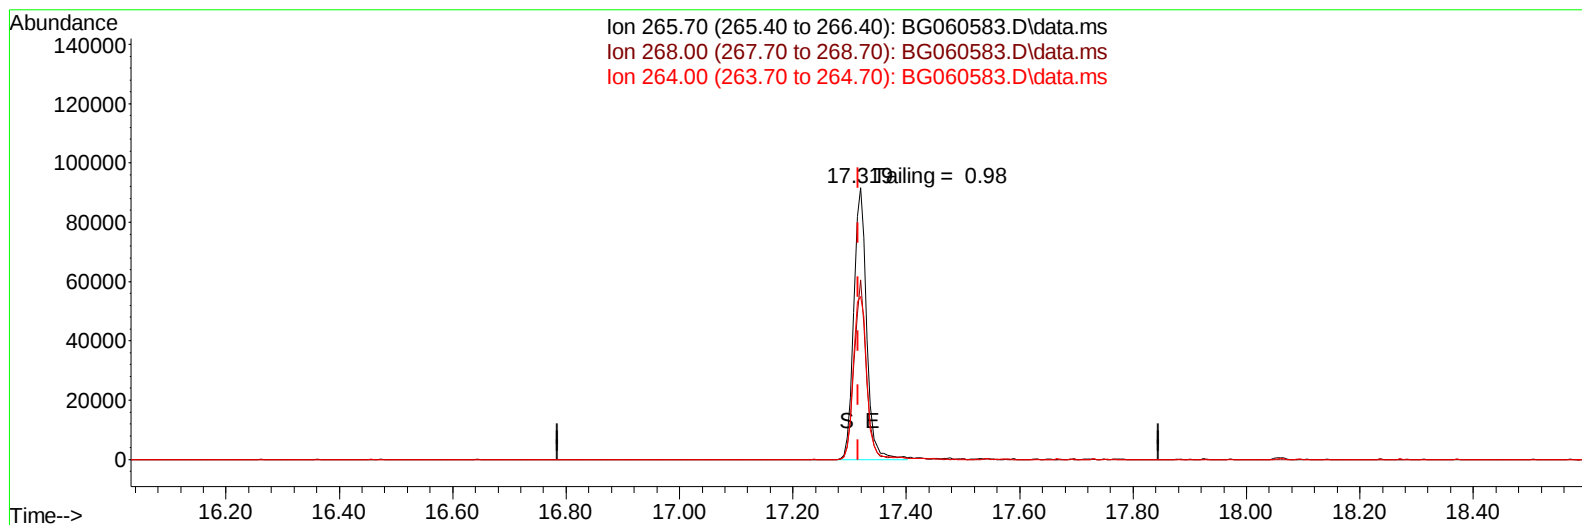

TIC: BG060583.D\data.ms

(70) Pentachlorophenol (C)

17.319min (+ 0.004) 226292.47 ng




response 143526

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.19
264.00	61.50	60.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030724\
Data File : BG060583.D
Acq On : 7 Mar 2024 10:34
Operator : MA/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Mar 08 03:42:12 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 08 03:35:45 2024
Response via : Initial Calibration

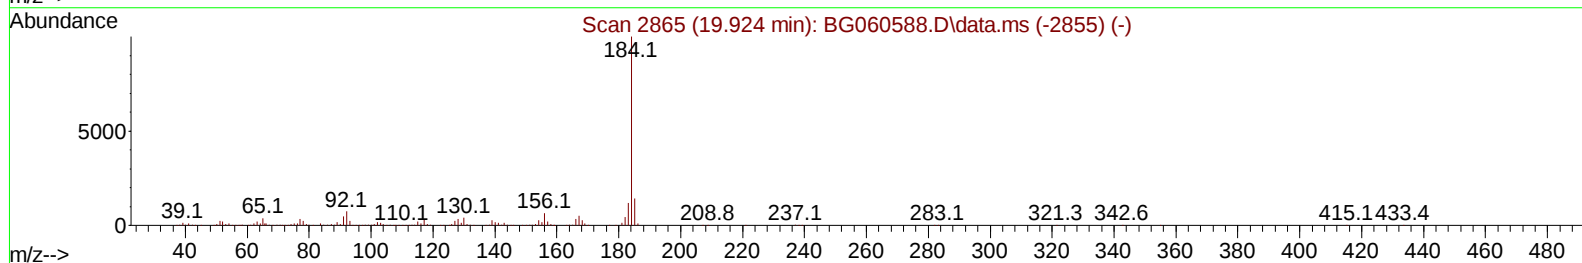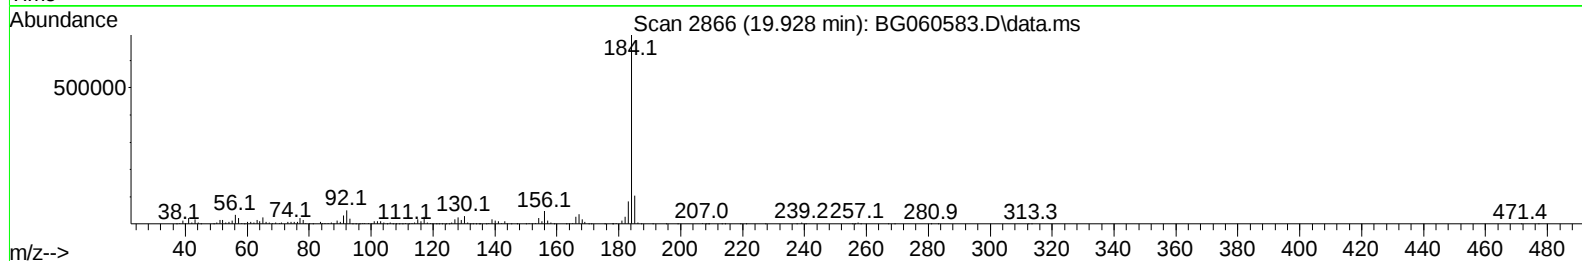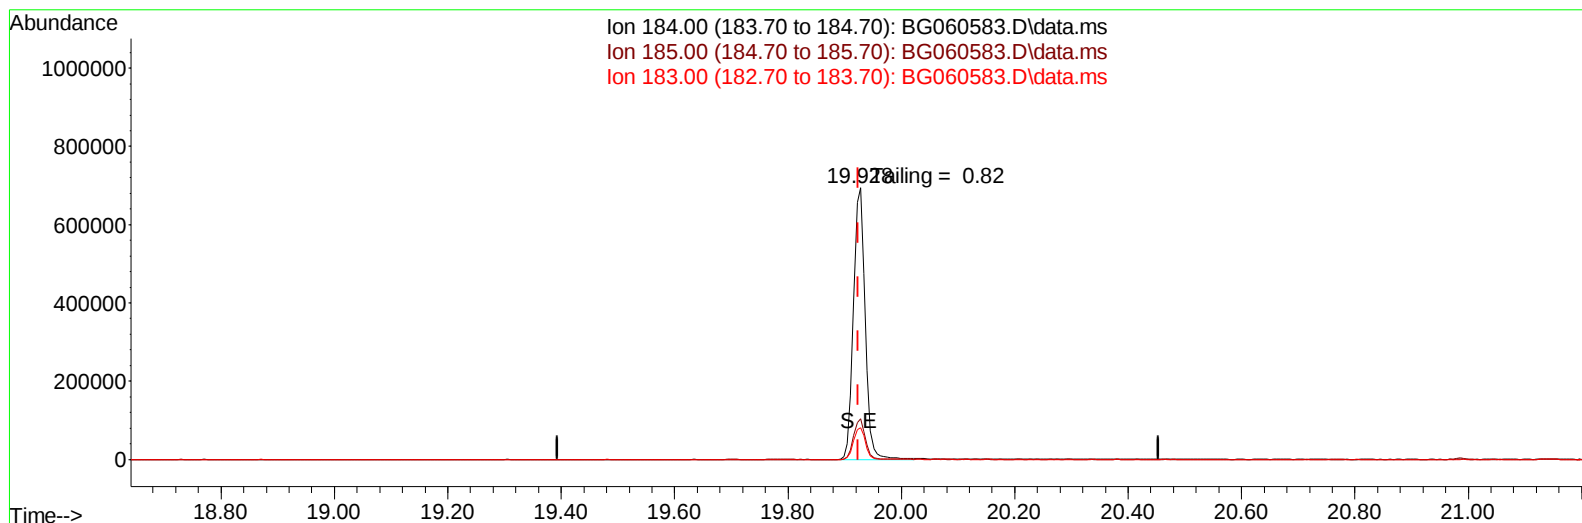

TIC: BG060583.D\data.ms

(77) Benzidine

19.928min (+ 0.004) 526933.95 ng

response 998411

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.88
183.00	11.90	11.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/7/2024	BNA_G	<u>BG060583.D</u>
Compound Name	Response	Retention Time
DDT	343647	21.144
DDD	7493	20.68
DDE	0	20.117
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7493	351140	2.13

Instrument :
BNA_G
ClientSampleId :
DFTPP