
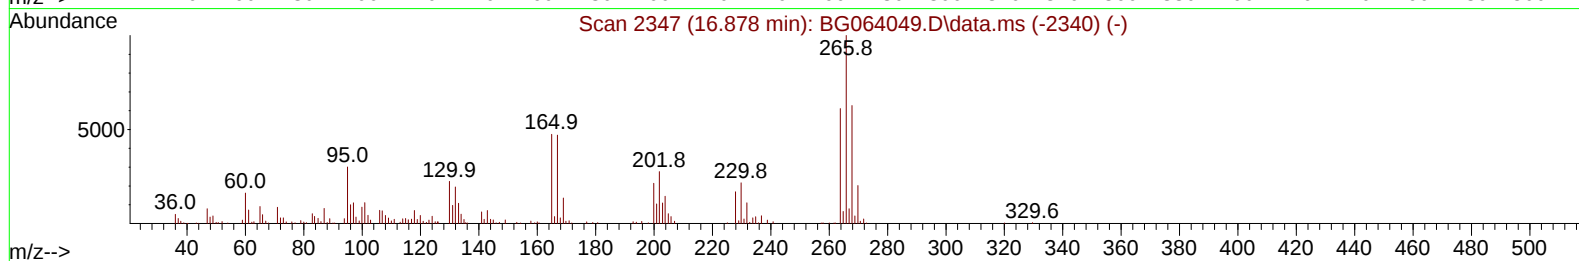
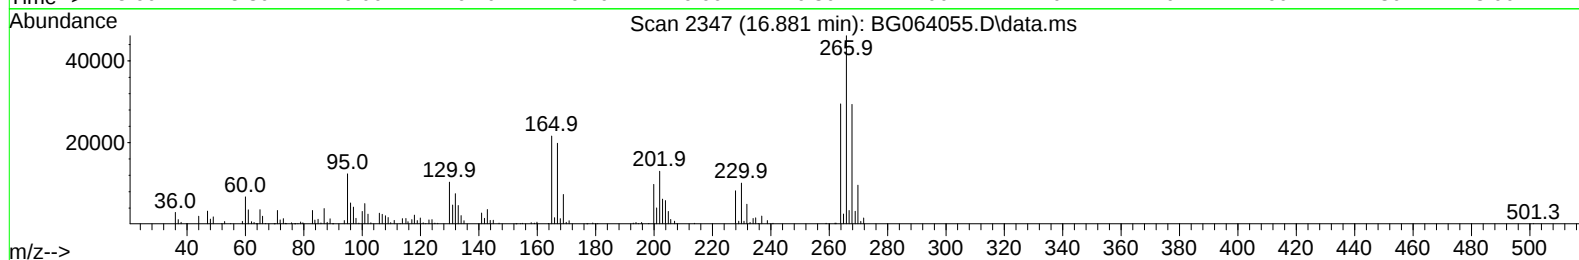


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030725\
Data File : BG064055.D
Acq On : 7 Mar 2025 12:15
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 07 14:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

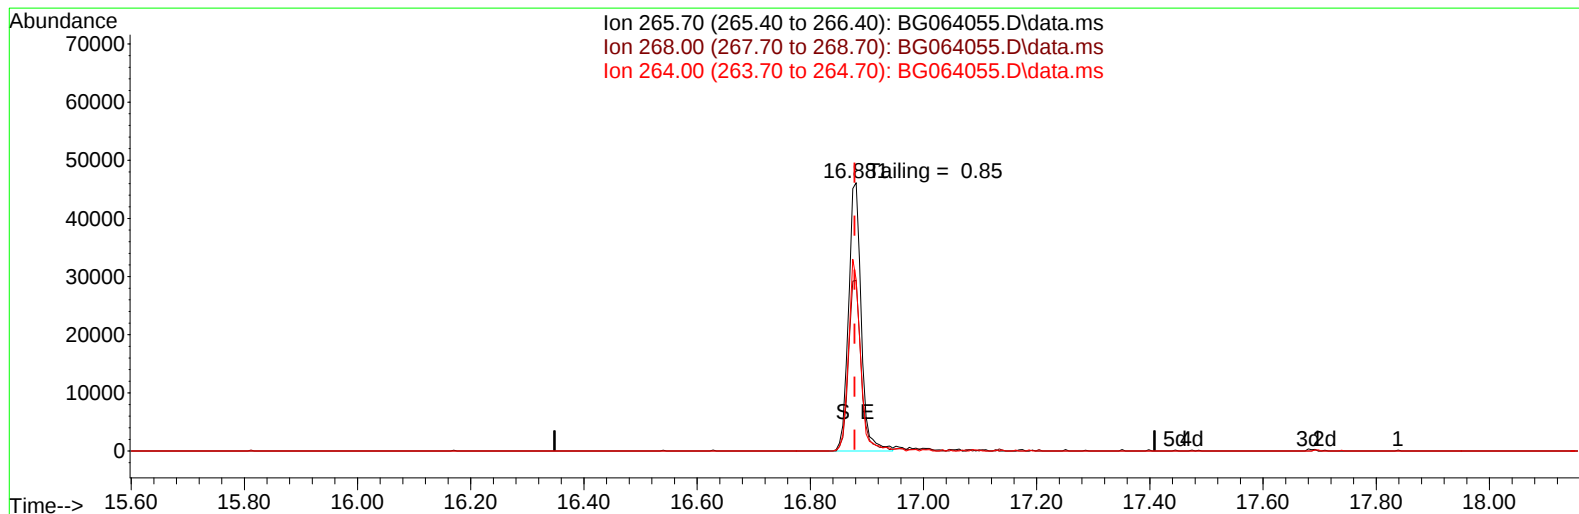

TIC: BG064055.D\data.ms




(70) Pentachlorophenol (C)

16.881min (+ 0.003) 140577.90 ng m

response 74060

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.80	63.59
264.00	61.10	63.88
0.00	0.00	0.00

Quant Time: Mar 07 14:17:51 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 05 15:39:19 2025
Response via : Initial Calibration

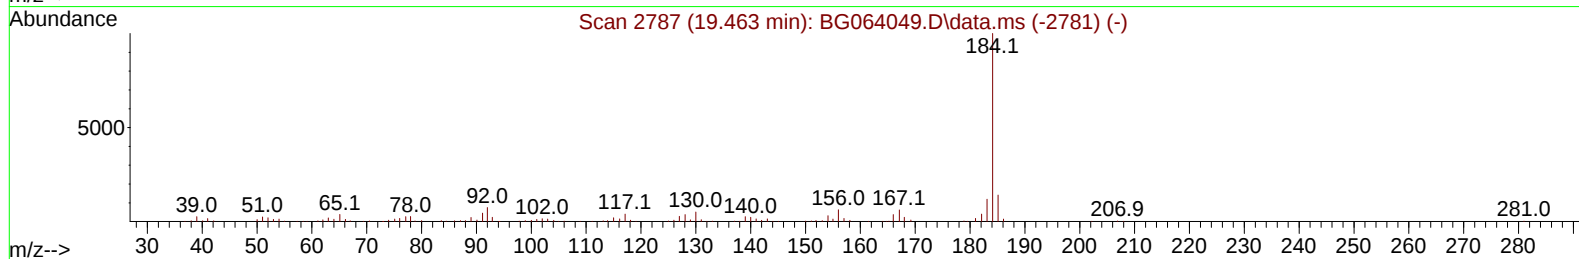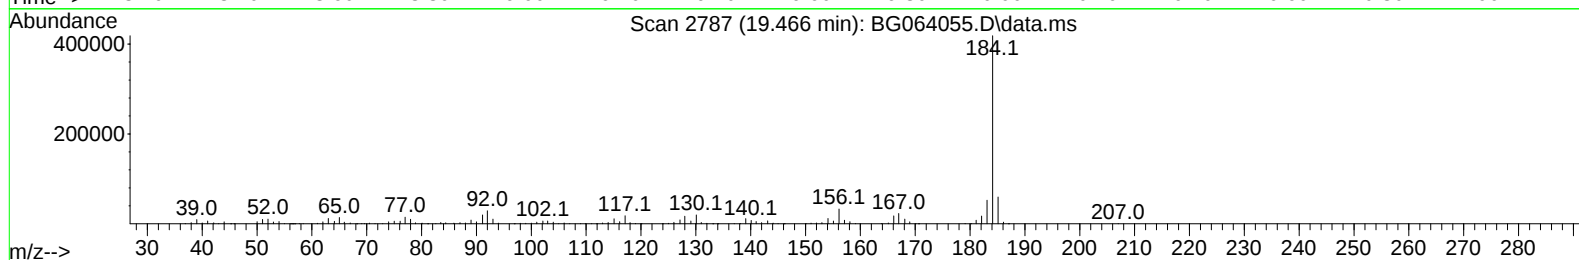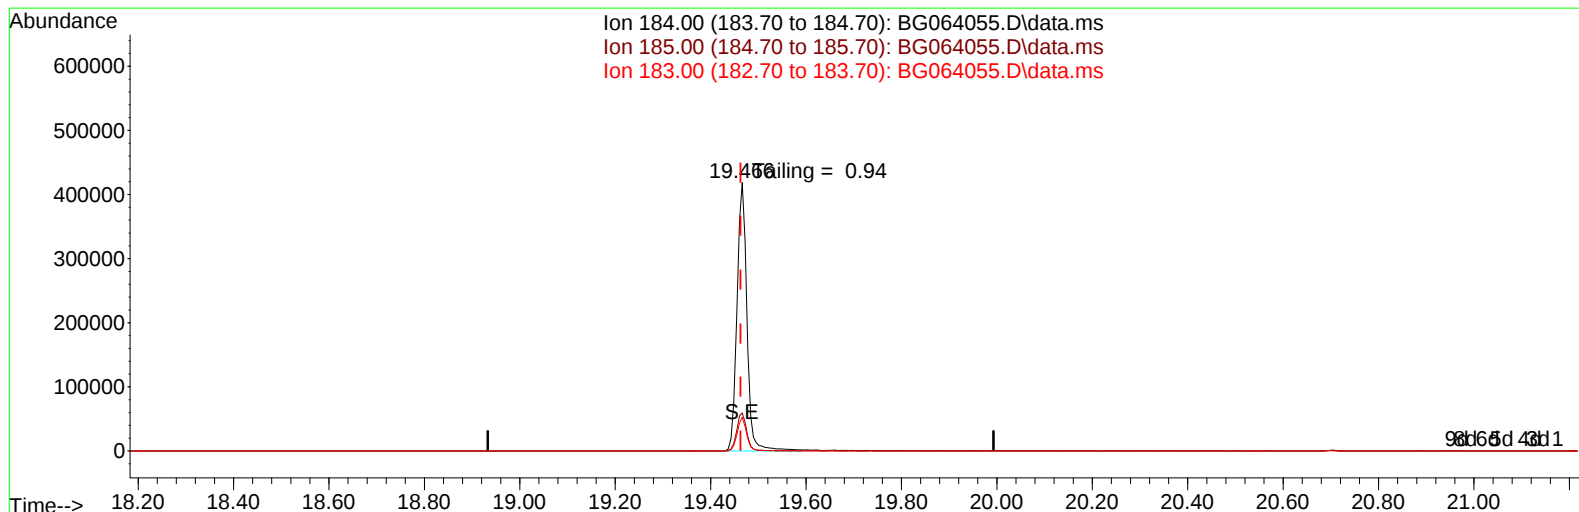

TIC: BG064055.D\data.ms

(77) Benzidine

19.466min (+ 0.003) 780316.23 ng m

response **626699**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.22
183.00	11.90	12.55
0.00	0.00	0.00