

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021361.D
 Acq On : 8 Mar 2016 11:16
 Operator : UM/SJ
 Sample : H1655-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-B280

Quant Time: Mar 09 00:14:48 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 00:13:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	10833	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	54198	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	32860	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	72783	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	75671	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	70591	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.53	96	1555	5.99	ng/uL	0.00
5) Phenol-d5	7.27	99	37576	33.07	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	25627	34.14	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	26474	33.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	30558	34.10	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	14305	32.99	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	15493	33.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	26288	31.86	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	36891	35.81	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	89808	33.06	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	116133	33.87	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	14751	27.57	ng/ul	0.00
58) Fluorene-d10	15.72	176	81407	33.81	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	12970	25.39	ng/ul	0.00
71) Anthracene-d10	17.57	188	125245	34.91	ng/ul	0.00
79) Pyrene-d10	19.84	212	134643	35.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	129989	34.60	ng/ul	0.00


Target Compounds					Qvalue
15) N-Nitroso-di-n-propylamine	8.82	70	1024	1.10 ng/ul#	1
45) Dimethylphthalate	14.18	163	13017	4.45 ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021361.D
Acq On : 8 Mar 2016 11:16
Operator : UM/SJ
Sample : H1655-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-B280

Quant Time: Mar 09 00:14:48 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 00:13:12 2016
Response via : Initial Calibration




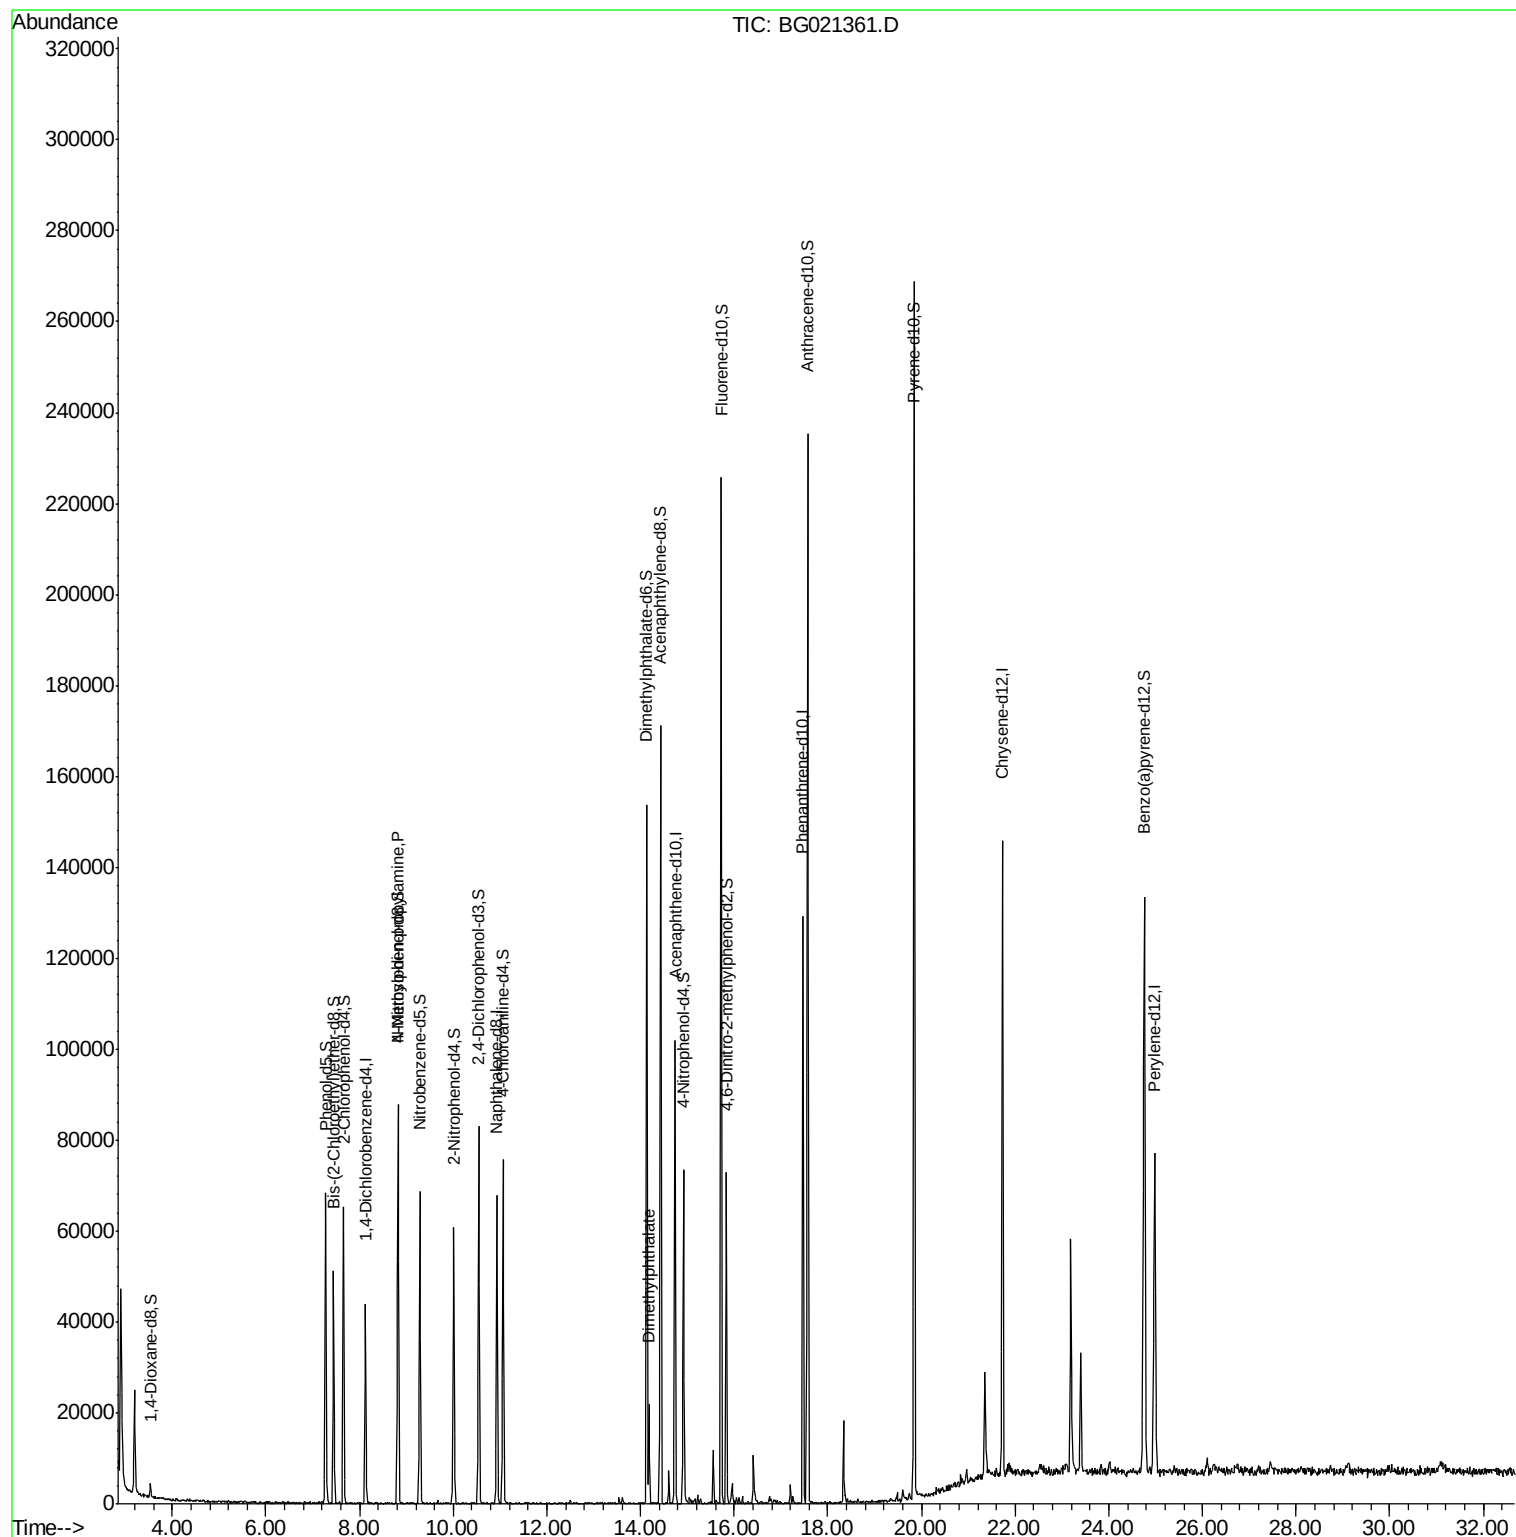


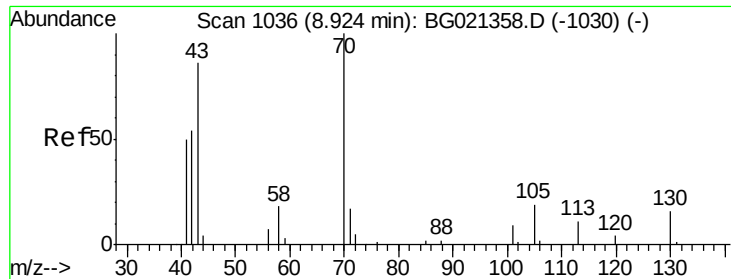

#15
N-Nitroso-di-n-propylamine
Concen: 1.10 ng/ul
RT: 8.82 min Scan# 1018
Delta R.T. -0.11 min
Lab File: BG021361.D
Acq: 8 Mar 2016 11:16

Instrument :
BNA_G
ClientSampleId :
MS-DS-B280

Tgt Ion: 70 Resp: 1024
Ion Ratio Lower Upper
70 100
42 348.6 45.7 68.5#
101 0.0 5.7 8.5#
130 0.0 15.7 23.5#

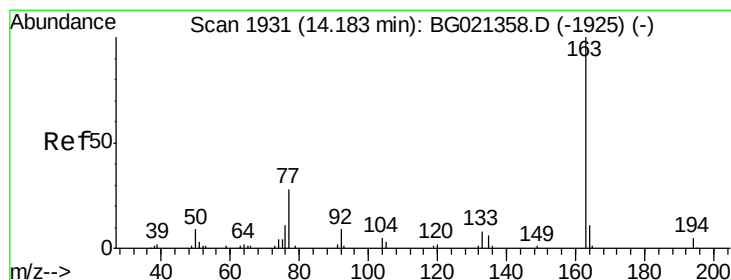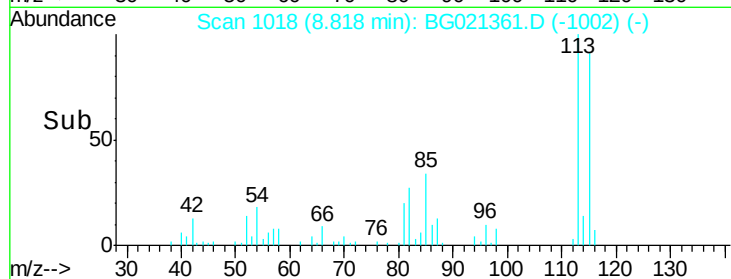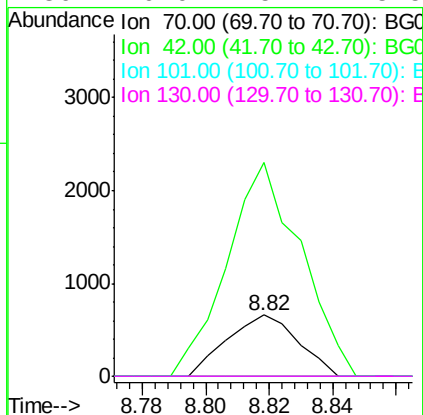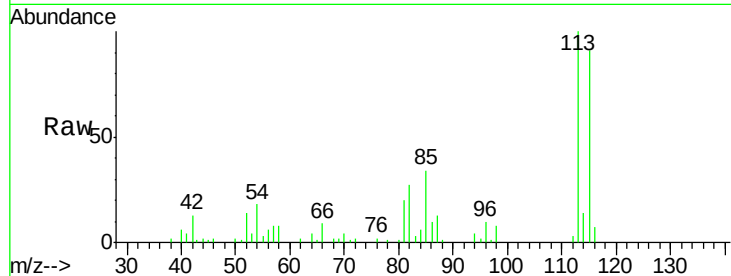

#45
Dimethylphthalate
Concen: 4.45 ng/ul
RT: 14.18 min Scan# 1930
Delta R.T. -0.01 min
Lab File: BG021361.D
Acq: 8 Mar 2016 11:16

Tgt Ion:163 Resp: 13017
Ion Ratio Lower Upper
163 100
194 3.9 2.8 4.2
164 10.3 8.2 12.2

