

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021367.D
 Acq On : 8 Mar 2016 15:13
 Operator : UM/SJ
 Sample : H1655-12
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-SS-B350

Quant Time: Mar 09 00:15:19 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 00:13:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	9825	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	49189	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	28766	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	67661	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	69893	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	64805	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	971	4.12	ng/uL	0.00
5) Phenol-d5	7.27	99	21053	20.43	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	14719	21.62	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	15390	21.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	16059	19.76	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	8248	20.96	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	8636	20.68	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	15338	20.49	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	21127	22.60	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	50273	21.14	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	64504	21.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	6957	14.85	ng/ul	0.00
58) Fluorene-d10	15.72	176	45606	21.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	6186	13.03	ng/ul	0.00
71) Anthracene-d10	17.57	188	69492	20.84	ng/ul	0.00
79) Pyrene-d10	19.84	212	72820	20.84	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.75	264	59453	17.24	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	9346	3.65	ng/ul#	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021367.D
Acq On : 8 Mar 2016 15:13
Operator : UM/SJ
Sample : H1655-12
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-SS-B350

Quant Time: Mar 09 00:15:19 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 00:13:12 2016
Response via : Initial Calibration

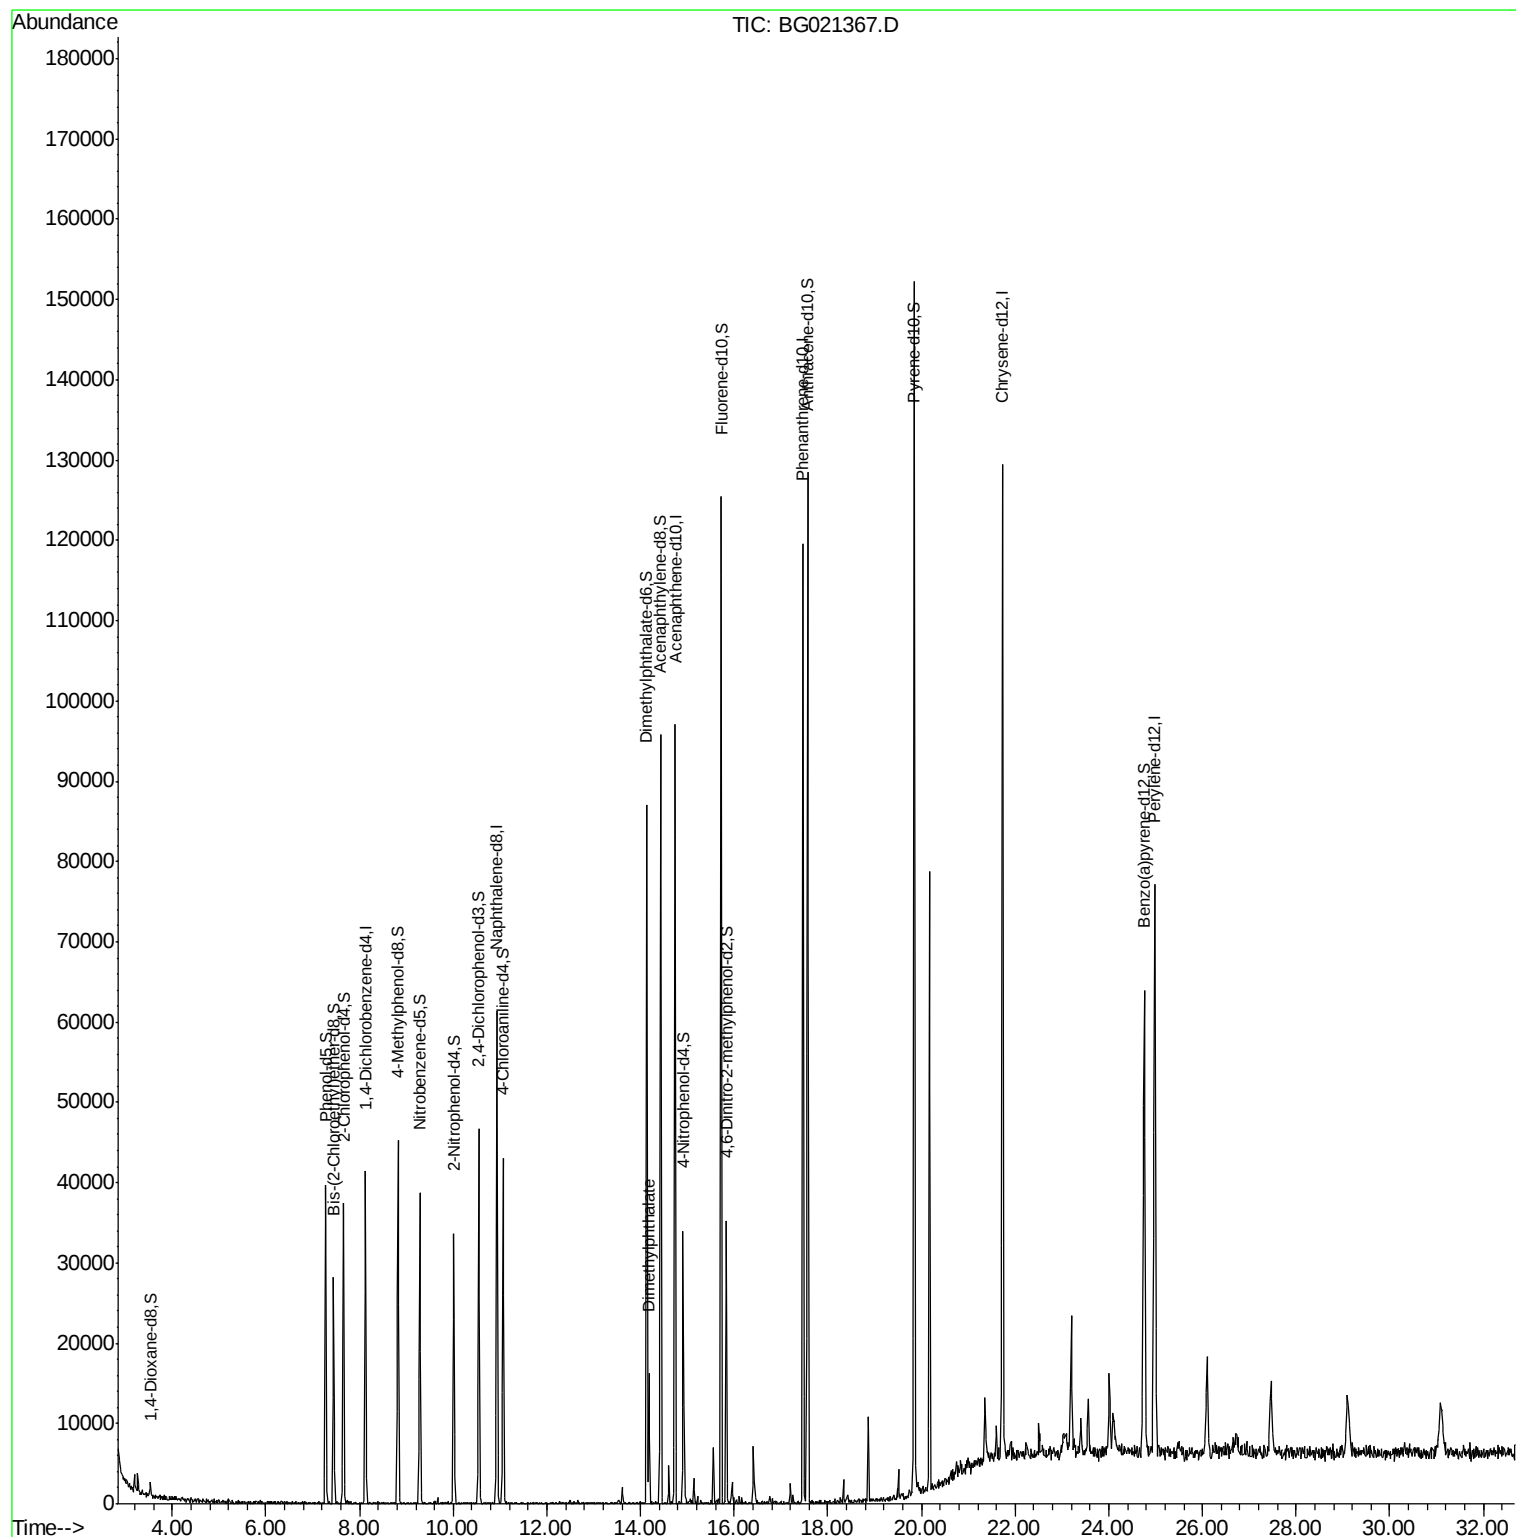

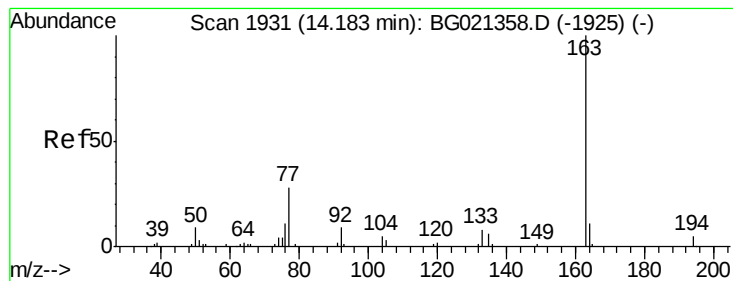

#45

Dimethylphthalate

Concen: 3.65 ng/ul

RT: 14.18 min Scan# 1930

Delta R.T. -0.01 min

Lab File: BG021367.D


Acq: 8 Mar 2016 15:13

Instrument :

BNA_G

ClientSampleId :

MS-SS-B350

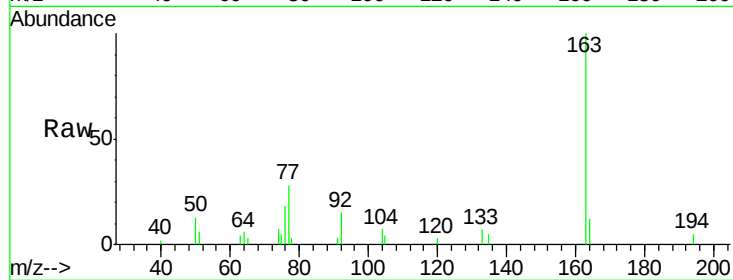

Tgt Ion:	163	Resp:	9346
Ion	Ratio	Lower	Upper
163	100		
194	5.5	2.8	4.2#
164	11.7	8.2	12.2

