

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021386.D
 Acq On : 9 Mar 2016 3:44
 Operator : UM/SJ
 Sample : H1625-07
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFF9

Quant Time: Mar 09 06:35:25 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 02:03:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	16623	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	86359	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	51586	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	92093	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	91032	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	86372	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	247	0.62	ng/uL	0.00
5) Phenol-d5	7.27	99	22498	12.90	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	14169	12.30	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	16692	13.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	18605	13.53	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	8734	12.64	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	8799	12.00	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	18103	13.77	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	4083	2.49	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	53017	12.43	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	74763	13.89	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	4980	5.93	ng/ul	0.00
58) Fluorene-d10	15.72	176	50608	13.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	3386	5.24	ng/ul	0.00
71) Anthracene-d10	17.57	188	64613	14.23	ng/ul	0.00
79) Pyrene-d10	19.85	212	66123	14.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.77	264	66301	14.43	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	18462	4.02	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021386.D
Acq On : 9 Mar 2016 3:44
Operator : UM/SJ
Sample : H1625-07
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFF9

Quant Time: Mar 09 06:35:25 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 02:03:52 2016
Response via : Initial Calibration

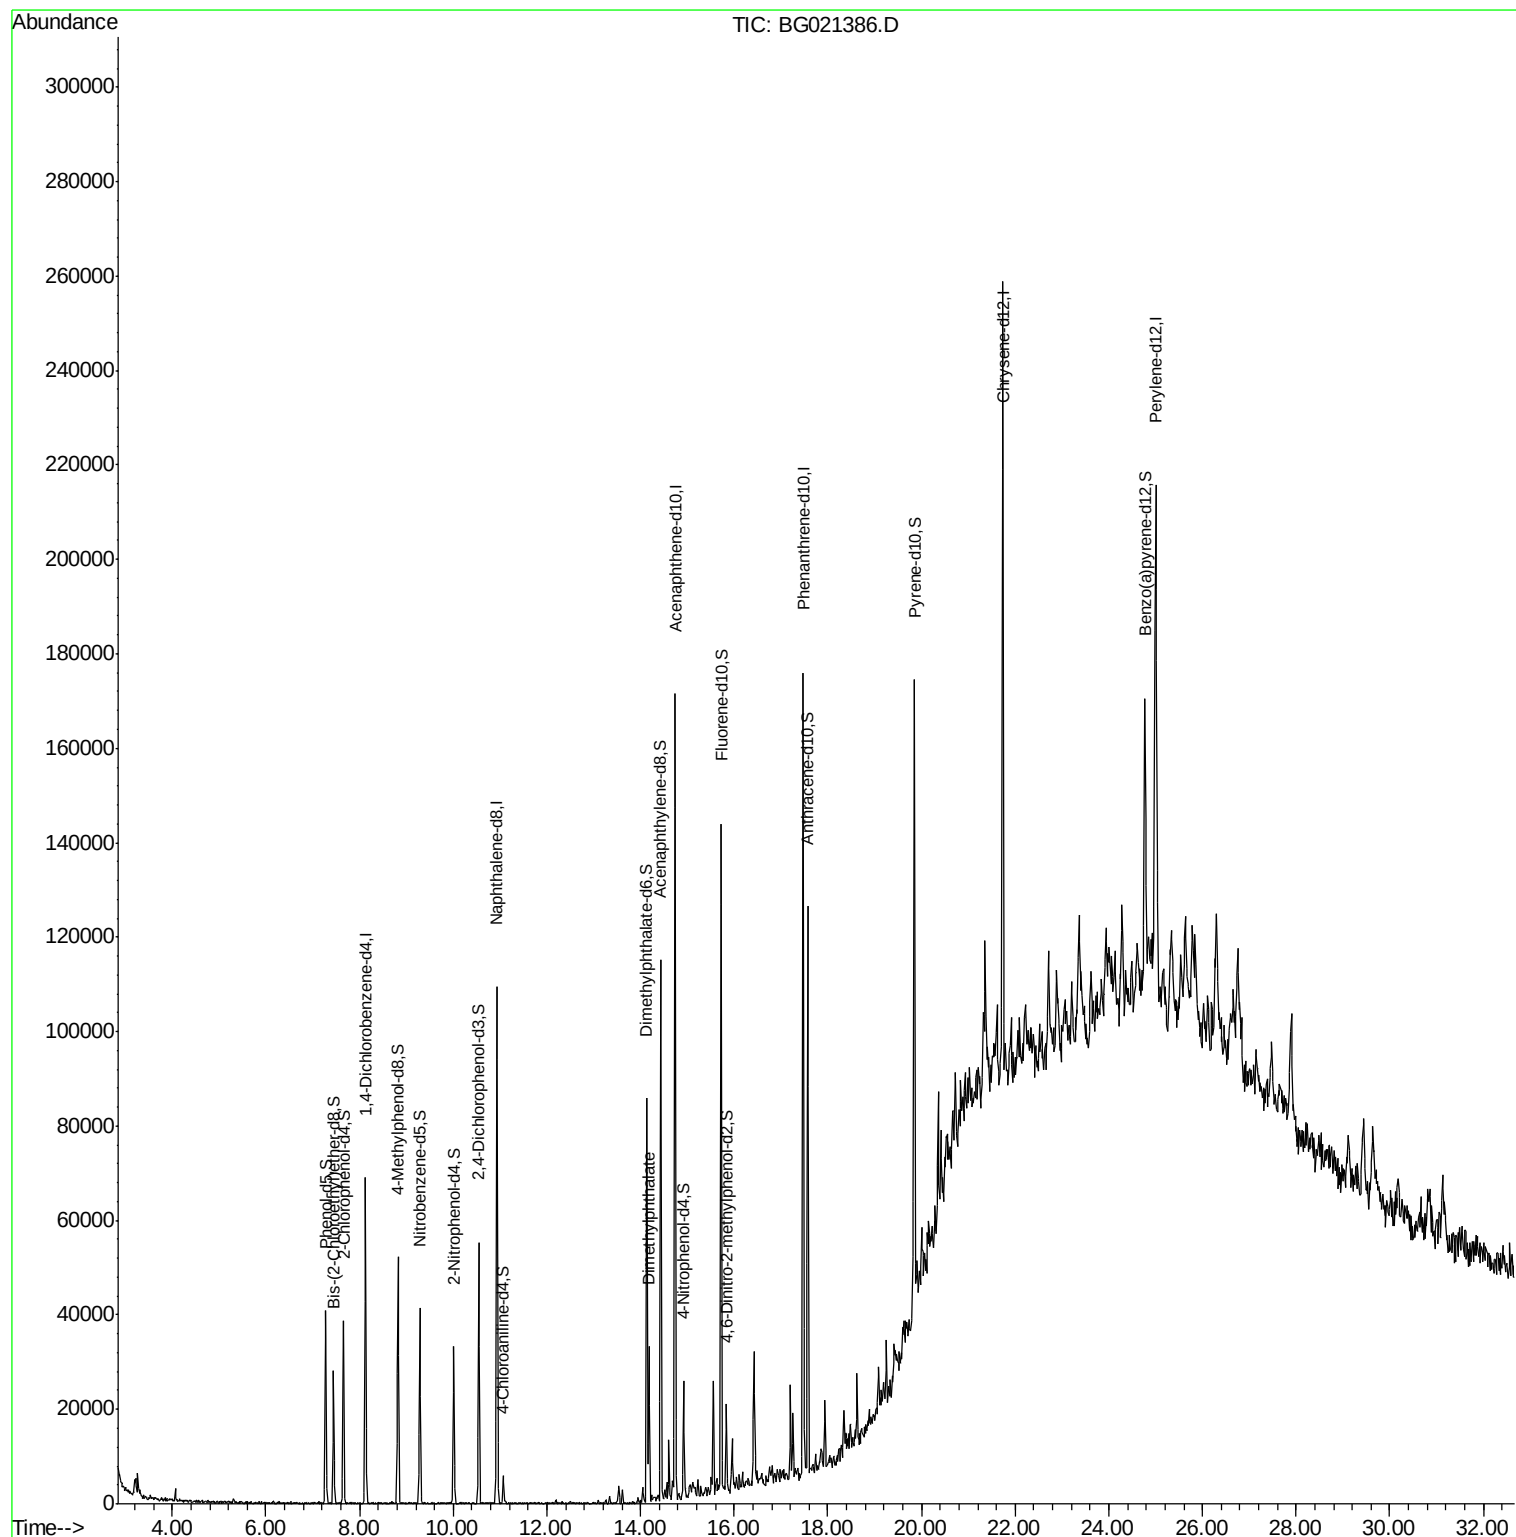

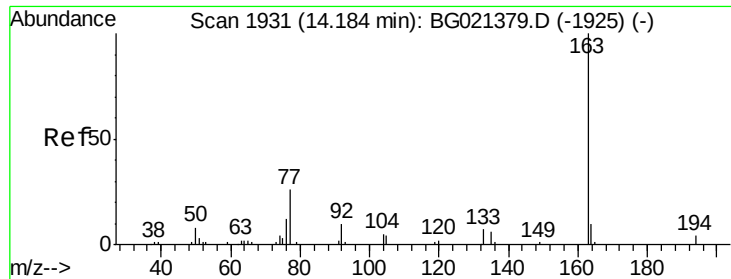

#45

Dimethylphthalate

Concen: 4.02 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. -0.00 min

Lab File: BG021386.D

Acq: 9 Mar 2016 3:44

Instrument :

BNA_G

ClientSampleId :

JHFF9


Tgt Ion:163 Resp: 18462

Ion Ratio Lower Upper

163 100

194 4.4 2.8 4.2#

164 8.8 8.2 12.2

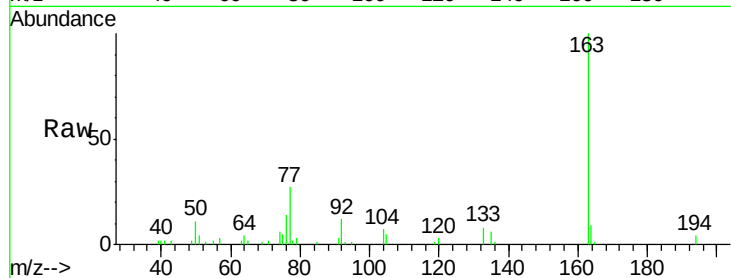

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

