

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021360.D
 Acq On : 8 Mar 2016 10:37
 Operator : UM/SJ
 Sample : H1655-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-C280

Quant Time: Mar 09 00:14:42 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 00:13:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10247	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	51281	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	31605	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	70471	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	73591	20.00	ng/ul	0.00
86) Perylene-d12	24.99	264	68548	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	1087	4.42	ng/uL	0.00
5) Phenol-d5	7.27	99	29129	27.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	20261	28.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	21717	28.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	24403	28.79	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	11450	27.91	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	11763	27.01	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	21337	27.33	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	31123	31.93	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	70121	26.83	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	91485	27.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.91	143	11212	21.79	ng/ul	0.00
58) Fluorene-d10	15.72	176	64312	27.77	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	10151	20.52	ng/ul	0.00
71) Anthracene-d10	17.57	188	98261	28.29	ng/ul	0.00
79) Pyrene-d10	19.84	212	108632	29.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	103882	28.48	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	17552	6.24	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021360.D
Acq On : 8 Mar 2016 10:37
Operator : UM/SJ
Sample : H1655-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-C280

Quant Time: Mar 09 00:14:42 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 00:13:12 2016
Response via : Initial Calibration

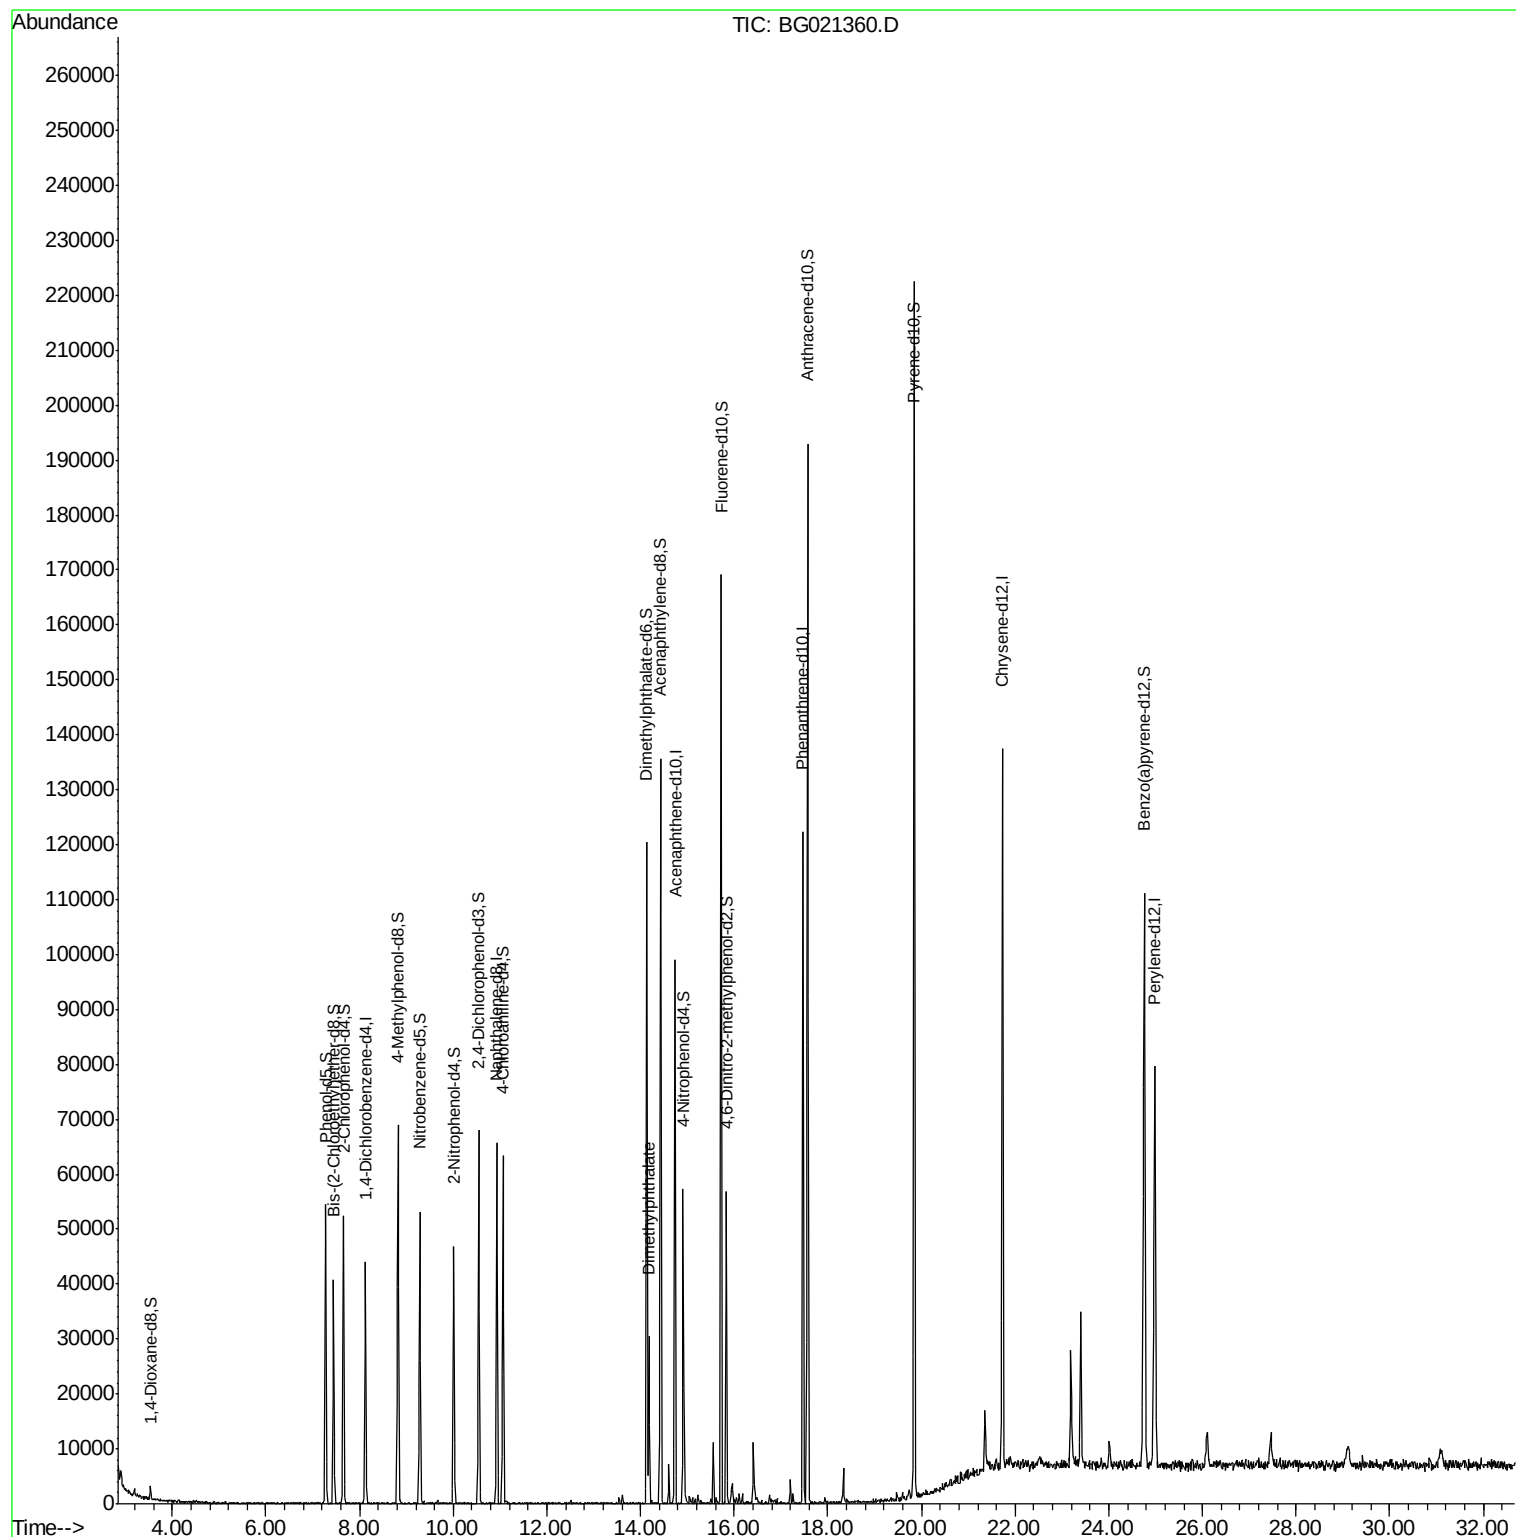


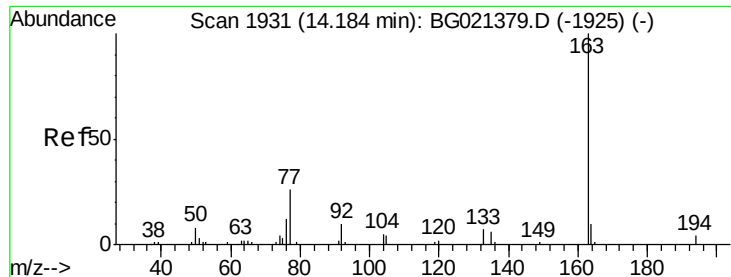

#45
 Dimethylphthalate
 Concen: 6.24 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG021360.D
 Acq: 8 Mar 2016 10:37

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-C280

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.2	2.8	4.2
164	12.2	8.2	12.2

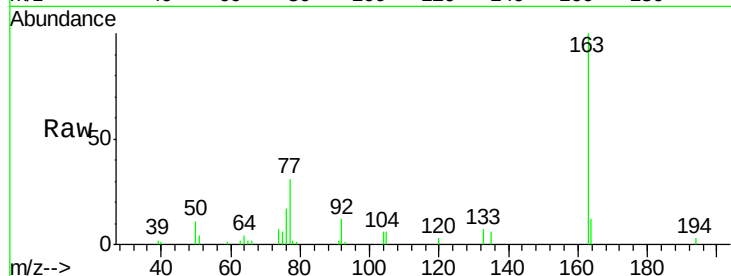

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

