

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021368.D
 Acq On : 8 Mar 2016 15:52
 Operator : UM/SJ
 Sample : H1655-13
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-B350

Quant Time: Mar 09 16:10:43 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 02:03:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	10250	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	50726	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	28859	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	65920	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	69117	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	65627	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1687	6.86	ng/uL	0.00
5) Phenol-d5	7.27	99	38970	36.25	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	27314	38.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	28274	37.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	31246	36.85	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	15235	37.54	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	15724	36.50	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	26726	34.61	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	39386	40.85	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	87263	36.57	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	113592	37.72	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15815	33.66	ng/ul	0.00
58) Fluorene-d10	15.72	176	78618	37.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	13145	28.41	ng/ul	0.00
71) Anthracene-d10	17.57	188	124630	38.35	ng/ul	0.00
79) Pyrene-d10	19.84	212	142993	41.39	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	136885	39.20	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	14663	5.71	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021368.D
Acq On : 8 Mar 2016 15:52
Operator : UM/SJ
Sample : H1655-13
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-B350

Quant Time: Mar 09 16:10:43 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 02:03:52 2016
Response via : Initial Calibration

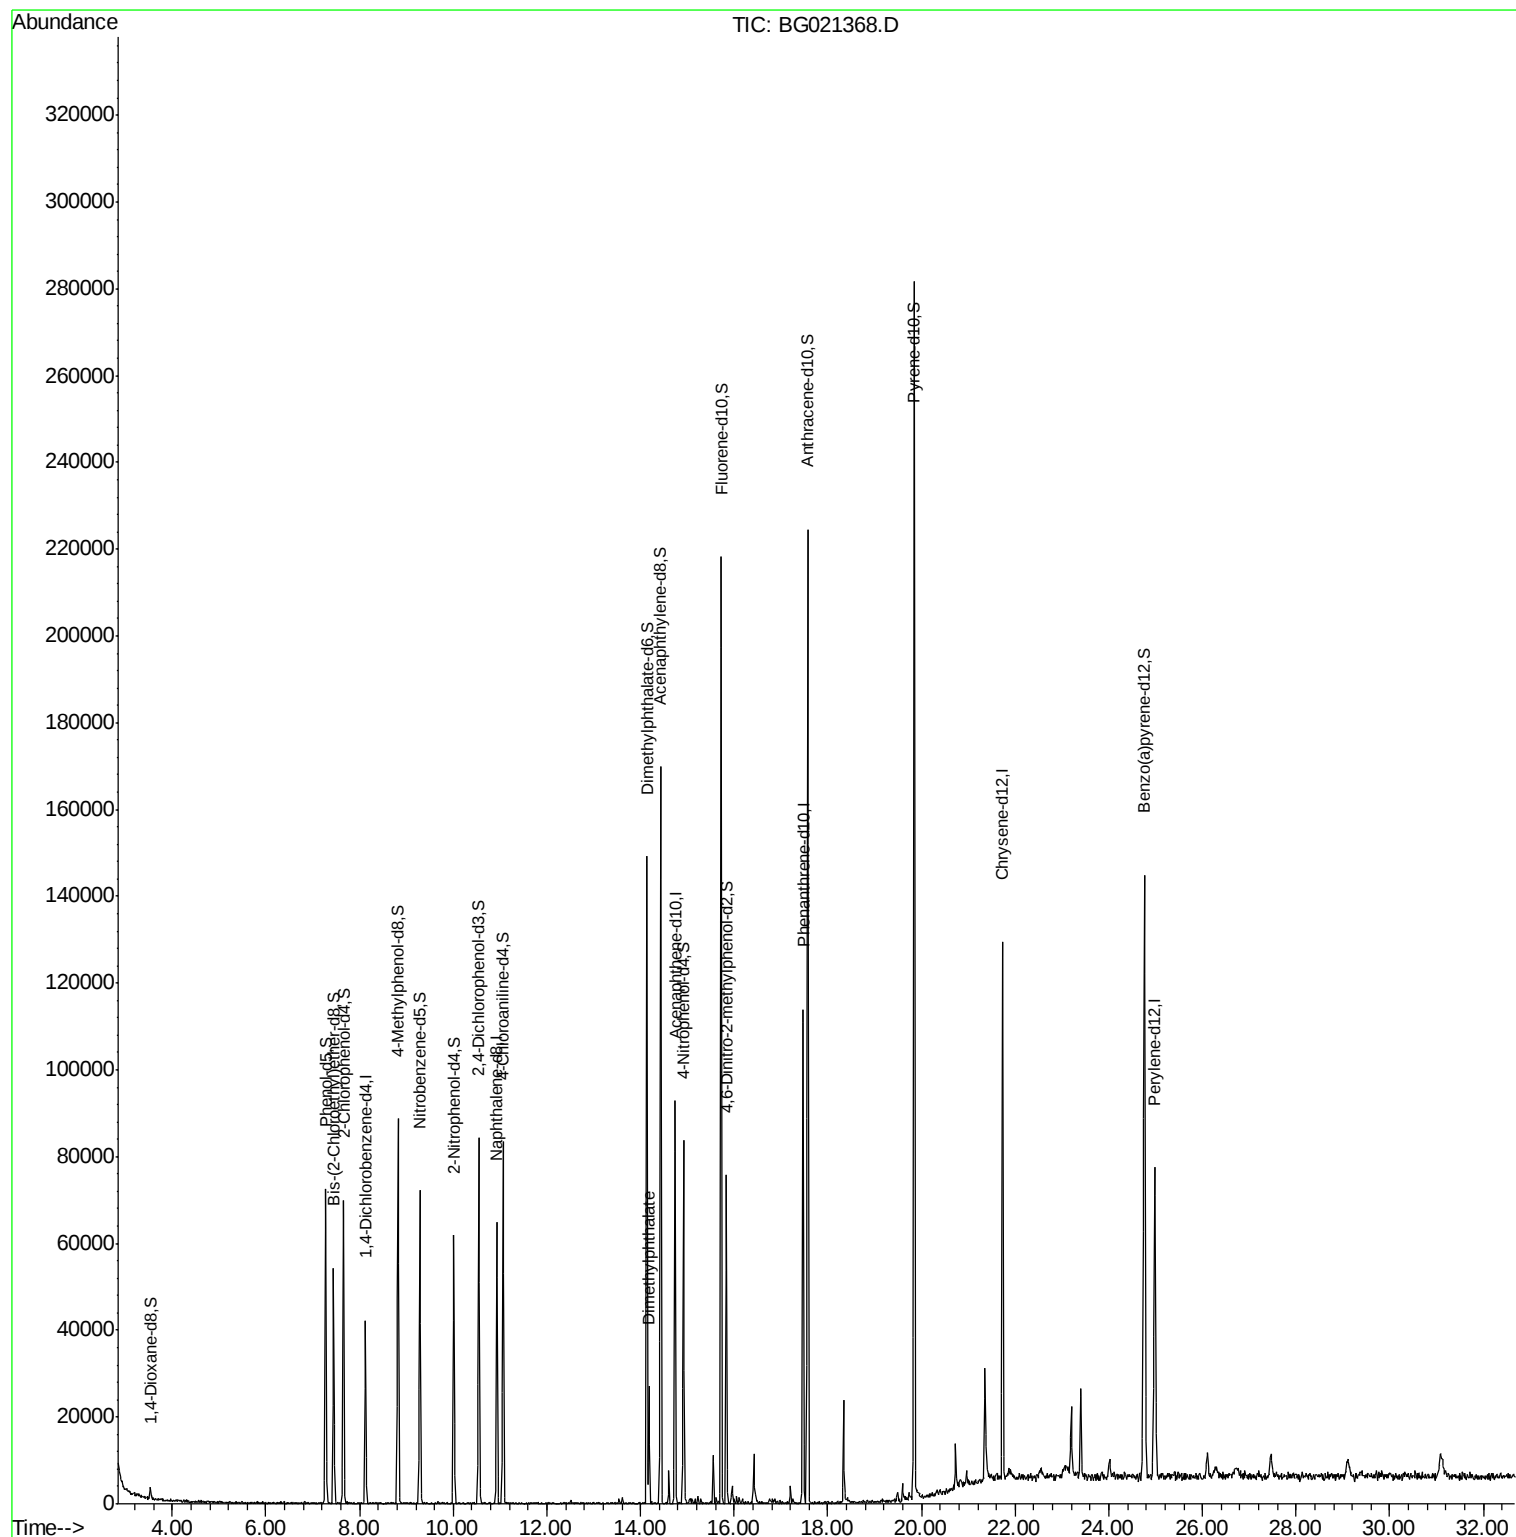


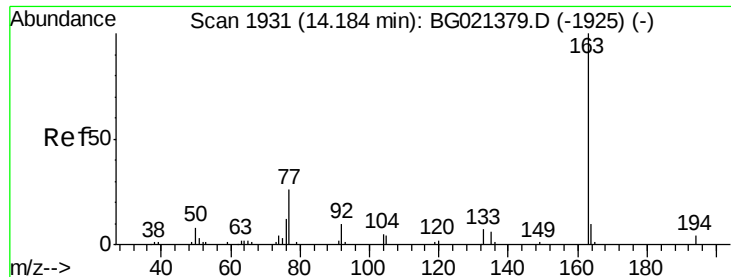

#45
 Dimethylphthalate
 Concen: 5.71 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.01 min
 Lab File: BG021368.D
 Acq: 8 Mar 2016 15:52

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-B350

Tgt Ion:	163	Resp:	14663
Ion	Ratio	Lower	Upper
163	100		
194	3.3	2.8	4.2
164	9.7	8.2	12.2

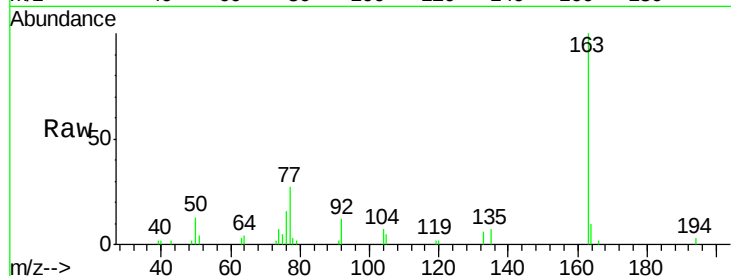

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

