

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021373.D
 Acq On : 8 Mar 2016 19:11
 Operator : UM/SJ
 Sample : H1655-15
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-E280

Quant Time: Mar 09 01:19:30 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 01:04:22 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.12	152	10083	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	49007	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.73	164	29315	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	67915	20.00	ng/ul	0.00
78) Chrysene-d12	21.73	240	72273	20.00	ng/ul	0.00
86) Perylene-d12	24.98	264	66331	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	1433	5.93	ng/uL	0.00
5) Phenol-d5	7.27	99	35938	33.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	25098	35.92	ng/ul	0.00
9) 2-Chlorophenol-d4	7.65	132	25967	35.20	ng/ul	0.00
13) 4-Methylphenol-d8	8.82	113	29524	35.39	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	13394	34.16	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	14788	35.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.54	165	25808	34.60	ng/ul	0.00
29) 4-Chloroaniline-d4	11.06	131	39778	42.70	ng/ul	0.00
44) Dimethylphthalate-d6	14.13	166	87642	36.16	ng/ul	0.00
47) Acenaphthylene-d8	14.43	160	111826	36.56	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	15241	31.93	ng/ul	0.00
58) Fluorene-d10	15.72	176	78423	36.51	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.83	200	12884	27.03	ng/ul	0.00
71) Anthracene-d10	17.57	188	124539	37.20	ng/ul	0.00
79) Pyrene-d10	19.84	212	137928	38.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.76	264	134503	38.11	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	21914	8.40	ng/ul#	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021373.D
Acq On : 8 Mar 2016 19:11
Operator : UM/SJ
Sample : H1655-15
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-DS-E280

Quant Time: Mar 09 01:19:30 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 01:04:22 2016
Response via : Initial Calibration

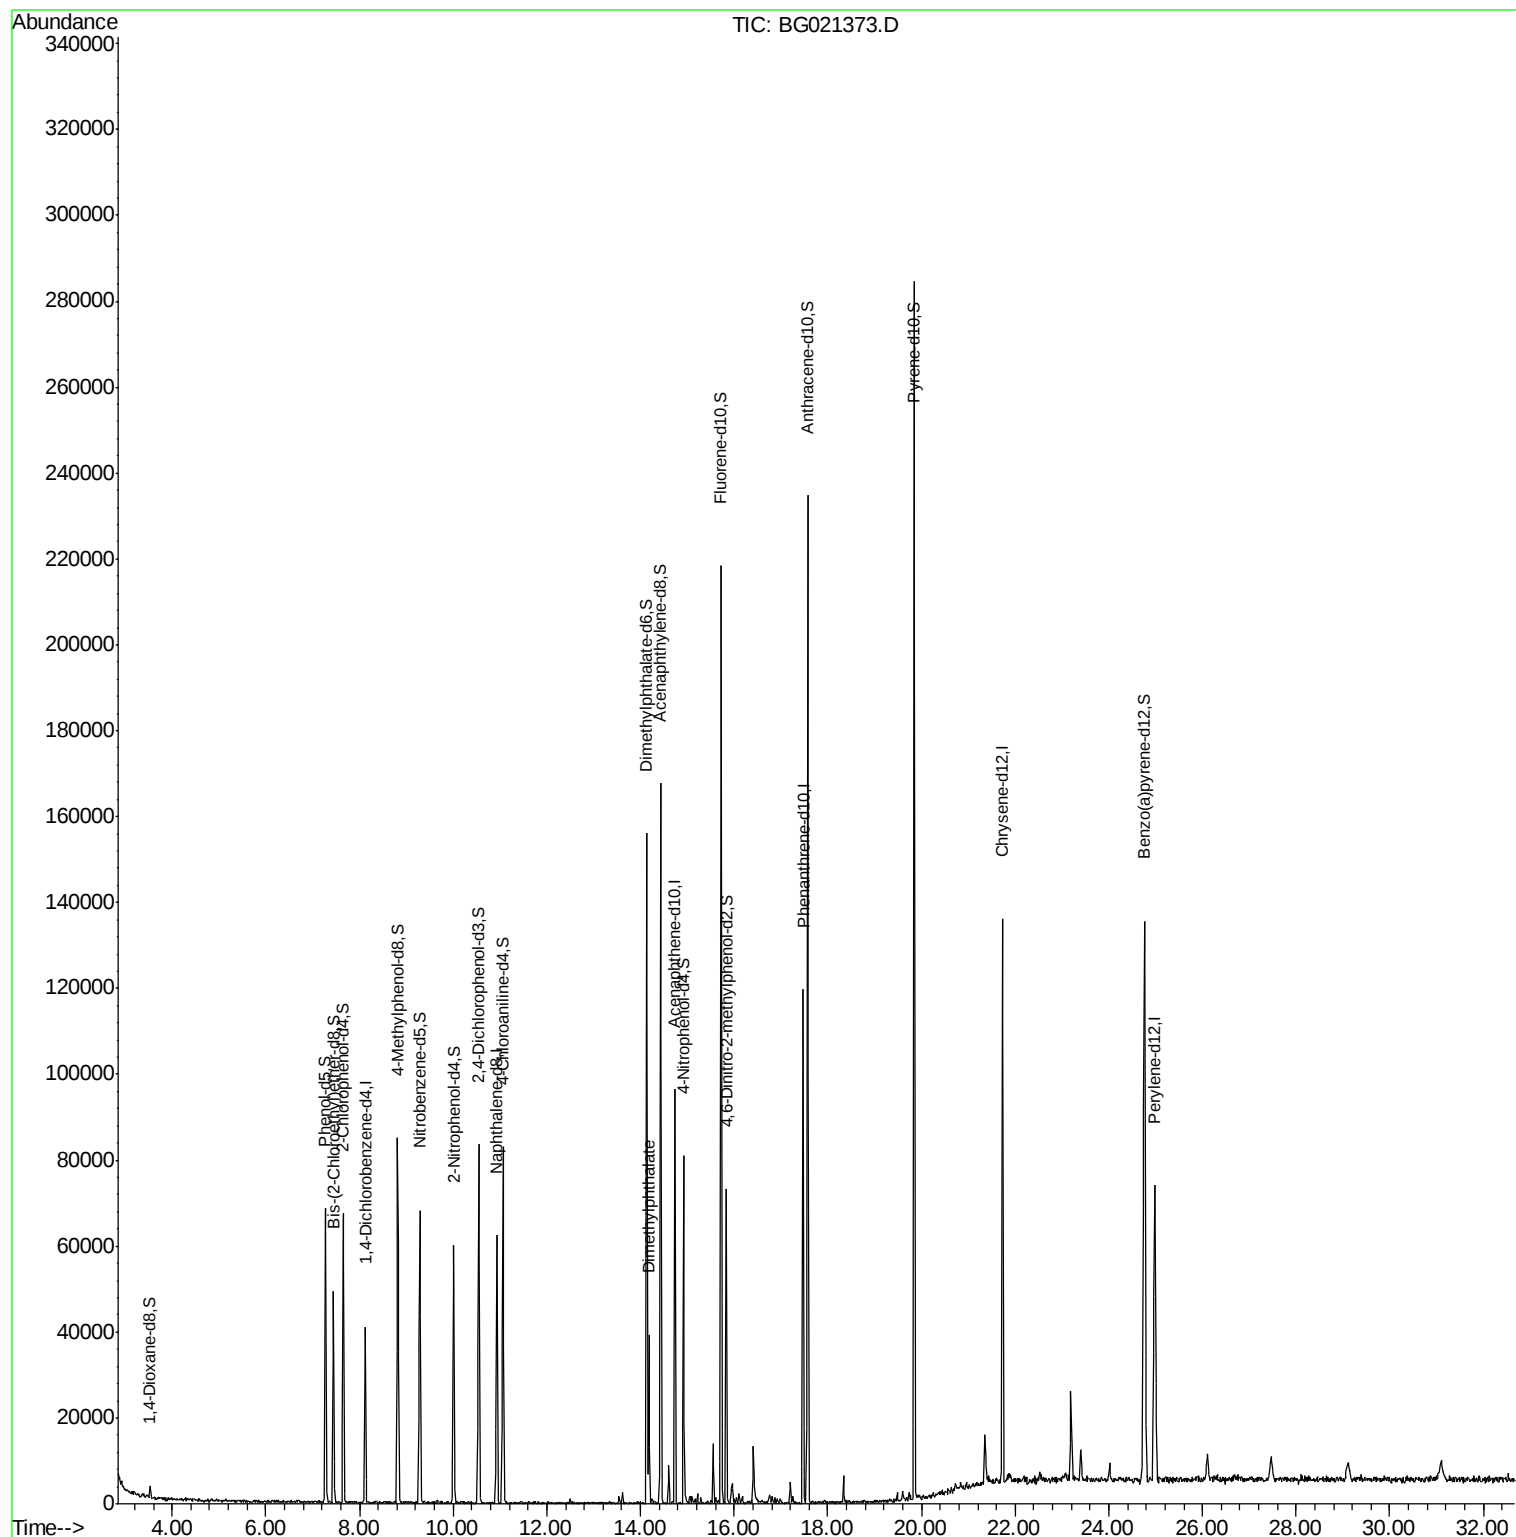


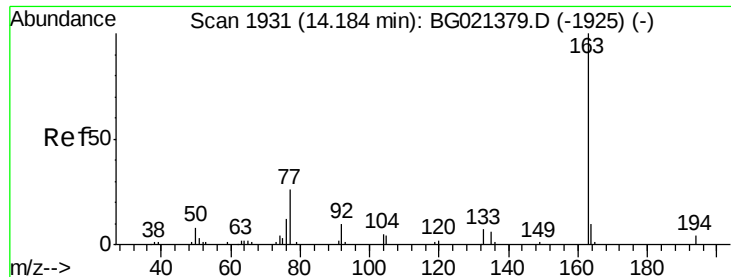

#45
 Dimethylphthalate
 Concen: 8.40 ng/ul
 RT: 14.18 min Scan# 1930
 Delta R.T. -0.00 min
 Lab File: BG021373.D
 Acq: 8 Mar 2016 19:11

Instrument :
 BNA_G
 ClientSampleId :
 MS-DS-E280

Tgt Ion:163 Resp: 21914
 Ion Ratio Lower Upper
 163 100
 194 4.5 2.8 4.2#
 164 10.6 8.2 12.2

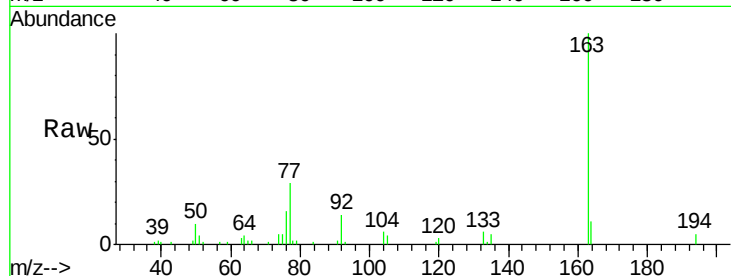

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

