

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021387.D
 Acq On : 9 Mar 2016 4:23
 Operator : UM/SJ
 Sample : H1625-08
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFG0

Quant Time: Mar 09 07:17:50 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 02:03:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	13716	20.00	ng/ul	0.00
18) Naphthalene-d8	10.93	136	65711	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	36787	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.47	188	76257	20.00	ng/ul	0.00
78) Chrysene-d12	21.74	240	85078	20.00	ng/ul	0.00
86) Perylene-d12	25.01	264	80300	20.00	ng/ul	0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.54	96	579	1.76	ng/uL	0.00
5) Phenol-d5	7.28	99	19152	13.31	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.44	67	13848	14.57	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	14866	14.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	14069	12.40	ng/ul	0.00
19) Nitrobenzene-d5	9.29	128	8126	15.46	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	7614	13.65	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	13953	13.95	ng/ul	0.00
29) 4-Chloroaniline-d4	11.07	131	8244	6.60	ng/ul	0.00
44) Dimethylphthalate-d6	14.14	166	41887	13.77	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	57836	15.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.92	143	4262	7.12	ng/ul	0.00
58) Fluorene-d10	15.72	176	40392	14.99	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.84	200	2984	5.58	ng/ul	0.00
71) Anthracene-d10	17.57	188	60194	16.01	ng/ul	0.00
79) Pyrene-d10	19.85	212	66650	15.67	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.78	264	66737	15.62	ng/ul	0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.18	163	15938	4.87	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021387.D
Acq On : 9 Mar 2016 4:23
Operator : UM/SJ
Sample : H1625-08
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFG0

Quant Time: Mar 09 07:17:50 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 02:03:52 2016
Response via : Initial Calibration

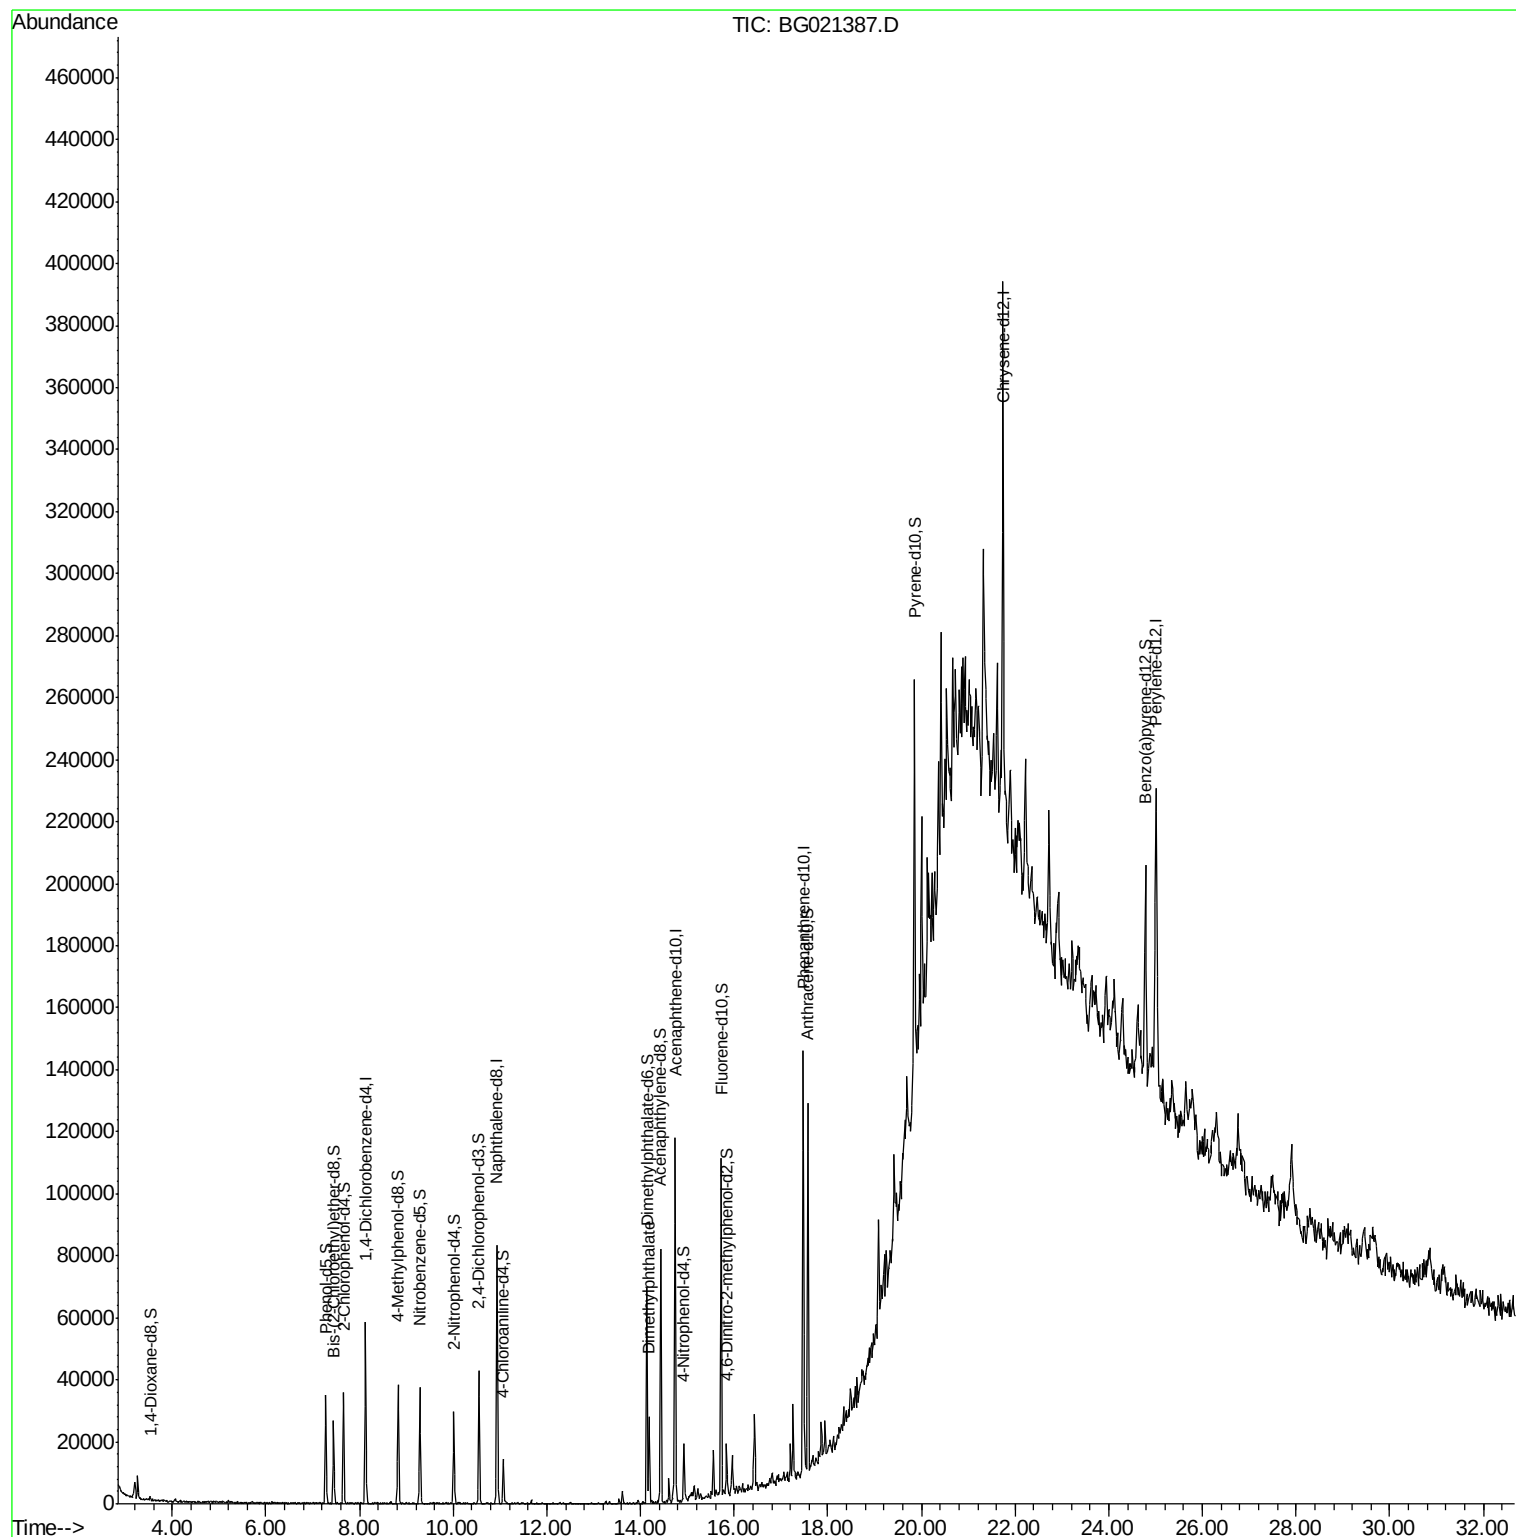

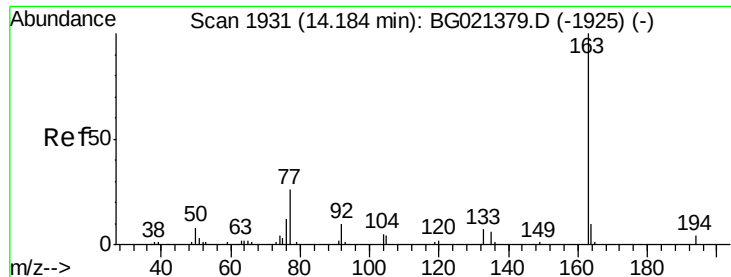

#45

Dimethylphthalate

Concen: 4.87 ng/ul

RT: 14.18 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BG021387.D


Acq: 9 Mar 2016 4:23

Instrument :

BNA_G

ClientSampleId :

JHFG0

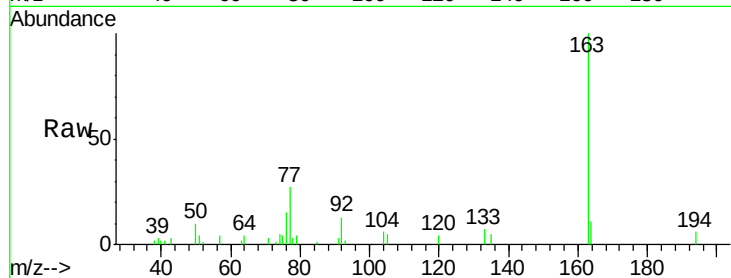

Tgt Ion:	163	Resp:	15938
Ion	Ratio	Lower	Upper
163	100		
194	5.5	2.8	4.2#
164	11.0	8.2	12.2

