

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021390.D
 Acq On : 9 Mar 2016 6:21
 Operator : UM/SJ
 Sample : H1625-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH2

Quant Time: Mar 09 10:05:24 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 09 02:03:52 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.13	152	15150	20.00	ng/ul	0.00
18) Naphthalene-d8	10.94	136	69904	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.74	164	40093	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.48	188	85193	20.00	ng/ul	0.00
78) Chrysene-d12	21.75	240	92358	20.00	ng/ul	0.01
86) Perylene-d12	25.02	264	85177	20.00	ng/ul	0.04

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.53	96	188	0.52	ng/uL	0.00
5) Phenol-d5	7.28	99	15637	9.84	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.45	67	12029	11.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.66	132	13242	11.95	ng/ul	0.00
13) 4-Methylphenol-d8	8.83	113	10240	8.17	ng/ul	0.00
19) Nitrobenzene-d5	9.30	128	7210	12.89	ng/ul	0.00
22) 2-Nitrophenol-d4	10.01	143	5824	9.81	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.55	165	11543	10.85	ng/ul	0.00
29) 4-Chloroaniline-d4	11.08	131	3933	2.96	ng/ul	0.01
44) Dimethylphthalate-d6	14.14	166	33771	10.19	ng/ul	0.00
47) Acenaphthylene-d8	14.44	160	56436	13.49	ng/ul	0.00
52) 4-Nitrophenol-d4	14.93	143	1832	2.81	ng/ul	0.01
58) Fluorene-d10	15.73	176	39299	13.38	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.85	200	339	0.57	ng/ul	0.02
71) Anthracene-d10	17.58	188	57383	13.66	ng/ul	0.01
79) Pyrene-d10	19.86	212	64076	13.88	ng/ul	0.01
90) Benzo(a)pyrene-d12	24.79	264	64377	14.20	ng/ul	0.03


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.19	163	15108	4.24	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021390.D
Acq On : 9 Mar 2016 6:21
Operator : UM/SJ
Sample : H1625-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH2

Quant Time: Mar 09 10:05:24 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 09 02:03:52 2016
Response via : Initial Calibration

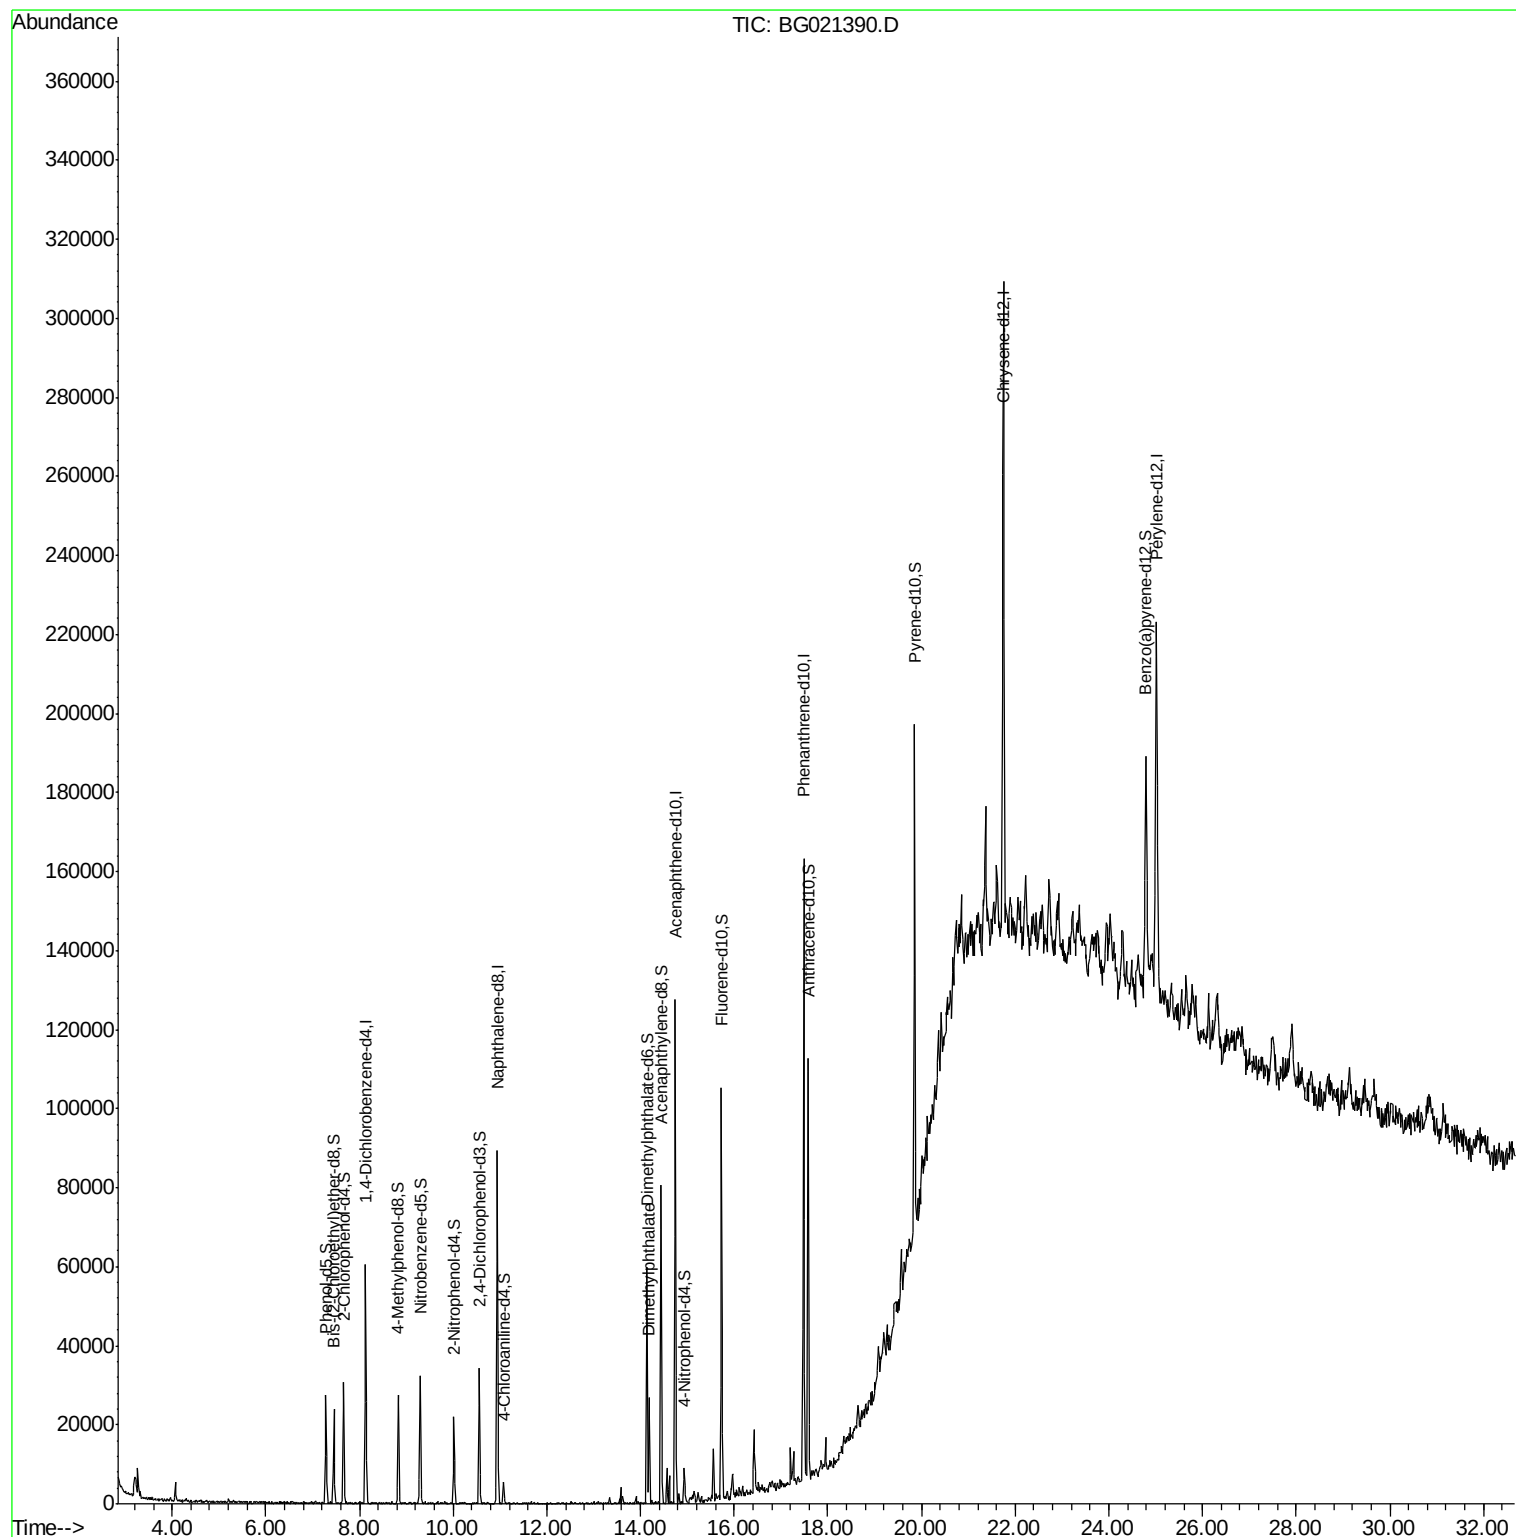

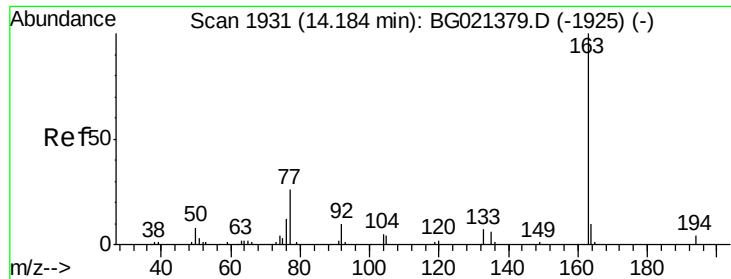

#45

Dimethylphthalate

Concen: 4.24 ng/ul

RT: 14.19 min Scan# 1931

Delta R.T. 0.00 min

Lab File: BG021390.D

Acq: 9 Mar 2016 6:21

Instrument :

BNA_G

ClientSampleId :

JHFH2


Tgt Ion:163 Resp: 15108

Ion Ratio Lower Upper

163 100

194 4.9 2.8 4.2#

164 8.8 8.2 12.2

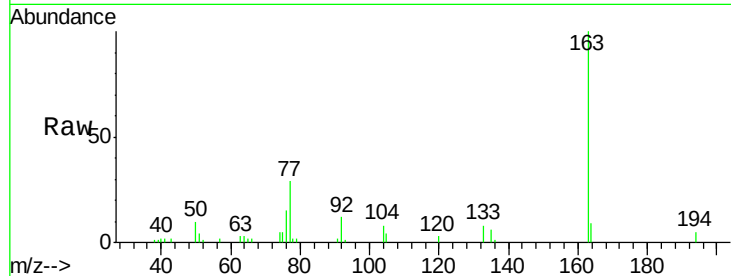

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

