

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
 Data File : BG021372.D
 Acq On : 8 Mar 2016 18:31
 Operator : UM/SJ
 Sample : PB88743BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.187	54	59	69	rVV2	13301	26592	7.40%	0.676%
2	3.263	69	72	76	rVB4	2689	3749	1.04%	0.095%
3	3.534	114	118	124	rVB	3497	5044	1.40%	0.128%
4	3.963	189	191	195	rBV2	495	546	0.15%	0.014%
5	4.245	236	239	241	rBV2	489	553	0.15%	0.014%
6	4.850	339	342	345	rBV	492	557	0.15%	0.014%
7	5.396	428	435	439	rBV2	473	1123	0.31%	0.029%
8	5.473	444	448	451	rVB2	371	570	0.16%	0.014%
9	5.661	476	480	484	rVB	388	546	0.15%	0.014%
10	5.984	532	535	540	rBV2	352	616	0.17%	0.016%
11	6.236	575	578	581	rVB	464	498	0.14%	0.013%
12	6.436	605	612	616	rBV2	379	825	0.23%	0.021%
13	6.789	670	672	675	rBV	486	525	0.15%	0.013%
14	6.953	698	700	703	rBB	425	491	0.14%	0.012%
15	7.271	749	754	765	rVV	66316	112259	31.22%	2.855%
16	7.341	765	766	771	rVB	539	539	0.15%	0.014%
17	7.447	776	784	792	rVB	49363	79646	22.15%	2.025%
18	7.652	810	819	826	rBV	66634	109659	30.50%	2.789%
19	7.917	860	864	867	rBV	575	751	0.21%	0.019%
20	8.122	892	899	909	rBV2	44351	74258	20.65%	1.888%
21	8.675	990	993	995	rBV	383	545	0.15%	0.014%
22	8.822	1012	1018	1026	rBV	80789	139897	38.91%	3.558%
23	8.875	1026	1027	1030	rVB	743	545	0.15%	0.014%
24	9.286	1091	1097	1105	rBB	66705	115597	32.15%	2.940%
25	9.597	1148	1150	1153	rBB	429	493	0.14%	0.013%
26	10.009	1212	1220	1228	rBV	57813	100832	28.04%	2.564%
27	10.543	1305	1311	1322	rBB	78355	137495	38.24%	3.497%
28	10.931	1370	1377	1385	rBB	65190	116395	32.37%	2.960%
29	11.066	1392	1400	1408	rBV	79401	143420	39.89%	3.647%
30	11.131	1408	1411	1413	rVB	515	506	0.14%	0.013%
31	12.500	1640	1644	1650	rBB2	811	1510	0.42%	0.038%
32	13.610	1830	1833	1838	rBB2	1954	2926	0.81%	0.074%
33	14.133	1916	1922	1928	rBV	148726	206231	57.36%	5.244%
34	14.433	1966	1973	1981	rBB	157788	244041	67.87%	6.206%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021372.D
Acq On : 8 Mar 2016 18:31
Operator : UM/SJ
Sample : PB88743BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 0.1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Title : SVOA CALIBRATION

35	14.732	2018	2024	2032	rVB2	96830	156852	43.62%	3.989%
36	14.915	2050	2055	2066	rBV2	77001	122534	34.08%	3.116%
37	15.044	2074	2077	2079	rVB	596	559	0.16%	0.014%
38	15.719	2186	2192	2200	rBB	201300	299392	83.27%	7.614%
39	15.831	2206	2211	2218	rVB	68061	94900	26.39%	2.413%
40	15.954	2229	2232	2236	rBV	1152	1456	0.40%	0.037%
41	17.470	2484	2490	2497	rBB	128299	187441	52.13%	4.767%
42	17.570	2500	2507	2514	rBV2	225798	327592	91.11%	8.331%
43	17.841	2551	2553	2556	rBV2	550	530	0.15%	0.013%
44	17.905	2563	2564	2567	rVB	755	489	0.14%	0.012%
45	18.222	2615	2618	2620	rVB	526	543	0.15%	0.014%
46	18.663	2690	2693	2698	rVB3	472	716	0.20%	0.018%
47	19.068	2761	2762	2766	rVB2	596	518	0.14%	0.013%
48	19.139	2770	2774	2778	rBV	345	567	0.16%	0.014%
49	19.474	2828	2831	2835	rBV2	1618	2108	0.59%	0.054%
50	19.621	2851	2856	2858	rBV	761	1112	0.31%	0.028%
51	19.732	2873	2875	2877	rVB2	1149	863	0.24%	0.022%
52	19.844	2887	2894	2900	rBV2	253543	359555	100.00%	9.144%
53	19.915	2904	2906	2908	rVB	1128	786	0.22%	0.020%
54	19.956	2911	2913	2915	rVB2	870	694	0.19%	0.018%
55	20.014	2921	2923	2925	rBV2	528	662	0.18%	0.017%
56	20.114	2939	2940	2945	rVB2	862	937	0.26%	0.024%
57	20.784	3053	3054	3057	rBV2	1208	978	0.27%	0.025%
58	21.730	3209	3215	3221	rVB	128950	209384	58.23%	5.325%
59	24.762	3722	3731	3741	rVB	124552	327032	90.95%	8.316%
60	24.985	3760	3769	3781	rVB3	72822	203277	56.54%	5.169%
61	25.855	3915	3917	3918	rBV2	1702	1078	0.30%	0.027%


Sum of corrected areas: 3932335

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021372.D
Acq On : 8 Mar 2016 18:31
Operator : UM/SJ
Sample : PB88743BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

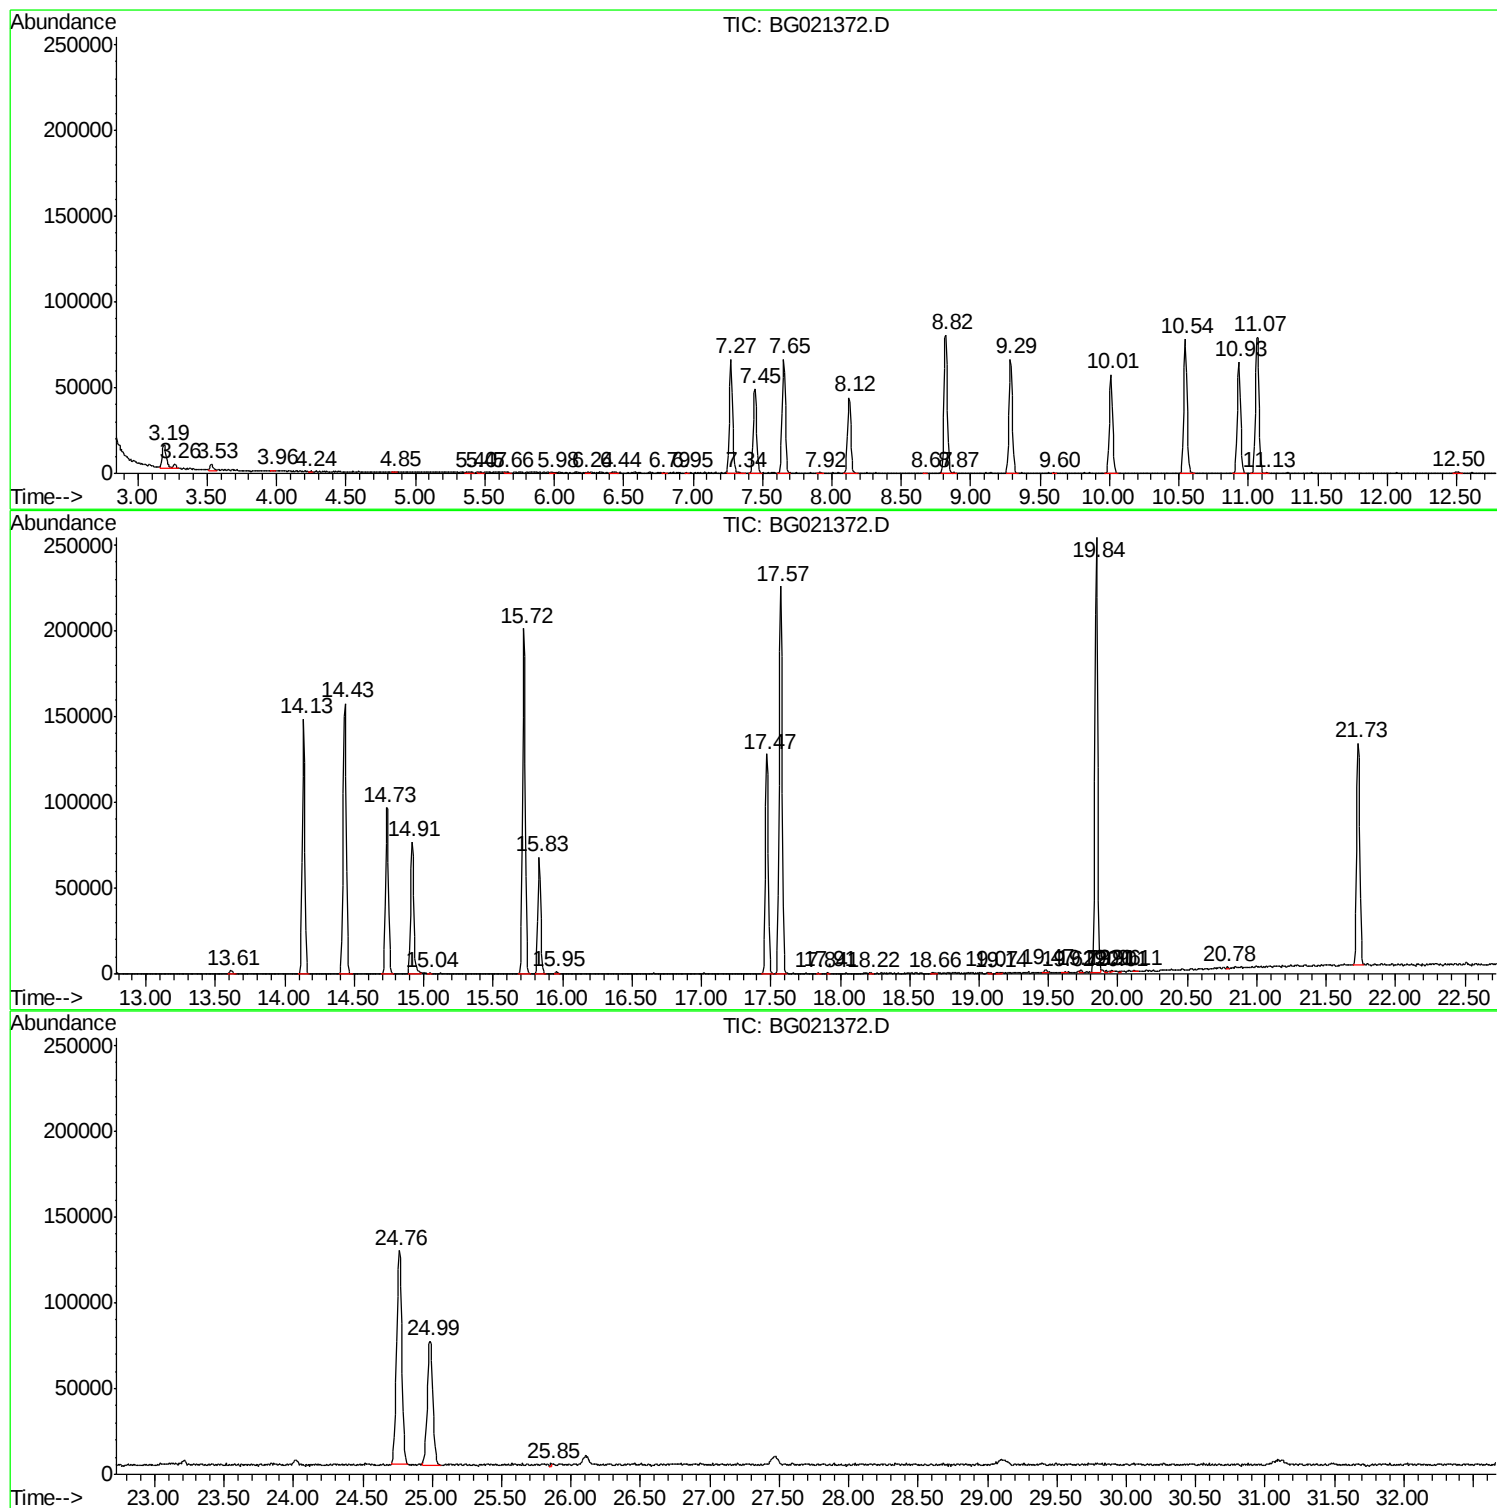

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021372.D
Acq On : 8 Mar 2016 18:31
Operator : UM/SJ
Sample : PB88743BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021372.D
Acq On : 8 Mar 2016 18:31
Operator : UM/SJ
Sample : PB88743BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
SBLK43

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc