

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021376.D
 Acq On : 8 Mar 2016 21:10
 Operator : UM/SJ
 Sample : H1705-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-GW-B350

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.531	117	118	122	rVB2	1139	938	0.24%	0.025%
2	3.566	122	124	127	rBV2	590	565	0.14%	0.015%
3	3.825	167	168	173	rBV2	744	873	0.22%	0.023%
4	3.960	186	191	192	rBV2	515	701	0.18%	0.019%
5	4.377	257	262	264	rBV2	460	788	0.20%	0.021%
6	4.653	306	309	311	rVB2	791	756	0.19%	0.020%
7	4.671	311	312	315	rBV2	563	535	0.13%	0.014%
8	4.894	348	350	355	rVB2	469	594	0.15%	0.016%
9	4.941	355	358	362	rBV3	615	788	0.20%	0.021%
10	5.452	442	445	450	rVB	368	590	0.15%	0.016%
11	5.699	482	487	491	rBV2	387	865	0.22%	0.023%
12	5.752	494	496	499	rBV	497	571	0.14%	0.015%
13	6.874	685	687	690	rVB	605	704	0.18%	0.019%
14	6.915	690	694	695	rBV	609	747	0.19%	0.020%
15	7.274	749	755	761	rBV2	17217	28502	7.16%	0.761%
16	7.444	777	784	793	rBV	47424	77009	19.34%	2.055%
17	7.650	813	819	827	rBV	54294	91270	22.92%	2.436%
18	8.126	894	900	906	rBV	41673	70282	17.65%	1.876%
19	8.625	983	985	988	rVB	612	554	0.14%	0.015%
20	8.819	1012	1018	1029	rVB2	50150	84545	21.23%	2.256%
21	8.901	1029	1032	1035	rBV2	460	727	0.18%	0.019%
22	9.289	1091	1098	1105	rBV	65819	117370	29.47%	3.132%
23	10.006	1213	1220	1227	rBV	59391	104425	26.22%	2.787%
24	10.547	1306	1312	1321	rVB	81863	141198	35.46%	3.768%
25	10.934	1371	1378	1385	rVB	64582	112588	28.27%	3.005%
26	11.064	1396	1400	1405	rBV2	2111	3250	0.82%	0.087%
27	12.503	1641	1645	1649	rBV3	1174	2001	0.50%	0.053%
28	13.613	1831	1834	1837	rBV	1081	1397	0.35%	0.037%
29	14.131	1915	1922	1929	rBB	152937	227440	57.11%	6.070%
30	14.430	1966	1973	1981	rBV	176740	269473	67.67%	7.192%
31	14.736	2018	2025	2034	rBB2	98412	151324	38.00%	4.039%
32	14.918	2051	2056	2063	rBV2	16358	27881	7.00%	0.744%
33	15.723	2185	2193	2201	rVB	222438	330764	83.06%	8.828%
34	15.829	2206	2211	2218	rBV	84634	121796	30.58%	3.251%

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
 Data File : BG021376.D
 Acq On : 8 Mar 2016 21:10
 Operator : UM/SJ
 Sample : H1705-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 MS-GW-B350

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

35	15.964	2230	2234	2237	rVB2	1624	1850	0.46%	0.049%
36	17.174	2437	2440	2442	rBB2	503	544	0.14%	0.015%
37	17.268	2453	2456	2460	rBV2	716	747	0.19%	0.020%
38	17.474	2484	2491	2498	rVB2	118198	180063	45.21%	4.806%
39	17.568	2501	2507	2516	rBV2	238333	357960	89.89%	9.554%
40	17.920	2565	2567	2570	rVB2	569	545	0.14%	0.015%
41	18.008	2578	2582	2585	rBV	537	851	0.21%	0.023%
42	18.067	2590	2592	2595	rBV	405	538	0.14%	0.014%
43	18.331	2634	2637	2640	rVB	1859	1833	0.46%	0.049%
44	18.461	2656	2659	2662	rBV	595	700	0.18%	0.019%
45	18.860	2721	2727	2732	rVB3	3565	5136	1.29%	0.137%
46	18.896	2732	2733	2736	rBV	859	672	0.17%	0.018%
47	18.943	2739	2741	2744	rBV	467	649	0.16%	0.017%
48	19.078	2761	2764	2766	rBV	728	596	0.15%	0.016%
49	19.371	2811	2814	2818	rVB2	482	870	0.22%	0.023%
50	19.436	2824	2825	2829	rVB2	793	649	0.16%	0.017%
51	19.483	2829	2833	2836	rBV	2258	3150	0.79%	0.084%
52	19.595	2847	2852	2858	rBV5	2982	4552	1.14%	0.121%
53	19.653	2858	2862	2864	rVV2	780	926	0.23%	0.025%
54	19.736	2873	2876	2881	rVB3	1821	2564	0.64%	0.068%
55	19.789	2881	2885	2887	rBV	951	1122	0.28%	0.030%
56	19.847	2888	2895	2903	rVV	278160	398242	100.00%	10.629%
57	19.953	2911	2913	2915	rBV2	1085	809	0.20%	0.022%
58	19.977	2915	2917	2919	rVV3	964	730	0.18%	0.019%
59	20.171	2944	2950	2956	rBV	24596	30053	7.55%	0.802%
60	20.218	2956	2958	2959	rBV	1000	546	0.14%	0.015%
61	20.388	2984	2987	2988	rBV2	1084	1115	0.28%	0.030%
62	20.406	2988	2990	2992	rVB2	1192	1016	0.26%	0.027%
63	20.523	3008	3010	3011	rBV	1143	630	0.16%	0.017%
64	20.594	3020	3022	3023	rBV	1008	536	0.13%	0.014%
65	20.952	3081	3083	3085	rBV3	1383	939	0.24%	0.025%
66	21.058	3099	3101	3103	rBV2	1678	1844	0.46%	0.049%
67	21.733	3209	3216	3223	rBV2	125801	212344	53.32%	5.667%
68	24.765	3722	3732	3741	rVB	141164	368565	92.55%	9.837%
69	24.988	3761	3770	3780	rVB2	68719	189186	47.51%	5.049%


Sum of corrected areas: 3746883

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021376.D
Acq On : 8 Mar 2016 21:10
Operator : UM/SJ
Sample : H1705-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-GW-B350

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

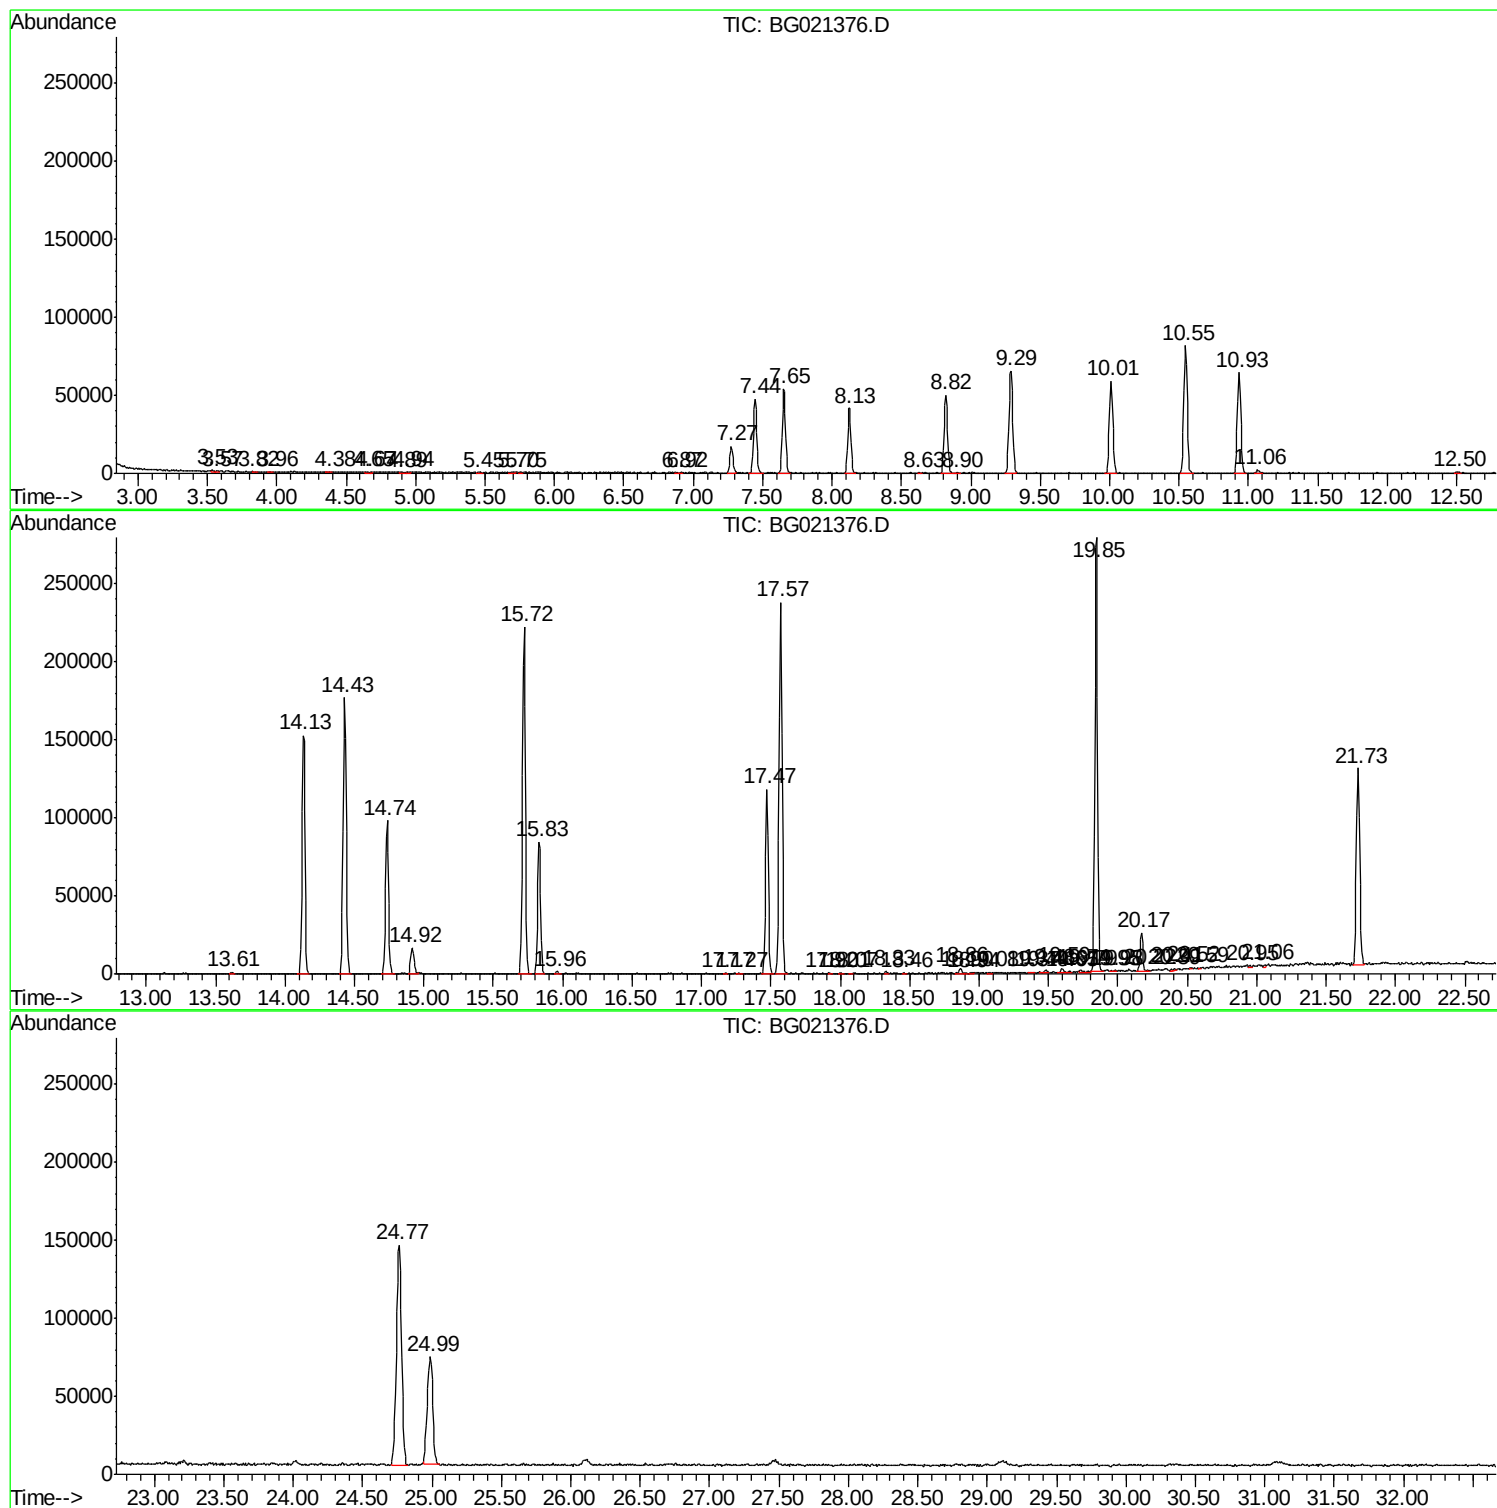

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021376.D
Acq On : 8 Mar 2016 21:10
Operator : UM/SJ
Sample : H1705-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-GW-B350

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030816\
Data File : BG021376.D
Acq On : 8 Mar 2016 21:10
Operator : UM/SJ
Sample : H1705-05
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
MS-GW-B350

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc