

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
 Data File : BG021390.D
 Acq On : 9 Mar 2016 6:21
 Operator : UM/SJ
 Sample : H1625-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.157	51	54	55	rBV2	461	587	0.22%	0.025%
2	3.193	55	60	63	rVV3	5009	10626	3.94%	0.455%
3	3.222	63	65	69	rVV2	4427	5797	2.15%	0.248%
4	3.263	69	72	76	rVV	7311	10246	3.80%	0.439%
5	3.316	78	81	86	rVB3	1870	2127	0.79%	0.091%
6	3.533	115	118	123	rVV2	512	726	0.27%	0.031%
7	3.598	128	129	132	rVB	551	467	0.17%	0.020%
8	3.633	132	135	138	rBV	366	538	0.20%	0.023%
9	3.868	171	175	177	rBV2	371	549	0.20%	0.024%
10	3.962	187	191	196	rBV3	814	1211	0.45%	0.052%
11	4.062	201	208	213	rBV	5011	7079	2.63%	0.303%
12	4.691	313	315	319	rBV2	446	743	0.28%	0.032%
13	5.208	400	403	406	rVB4	886	896	0.33%	0.038%
14	5.308	415	420	421	rBV	677	624	0.23%	0.027%
15	5.513	451	455	458	rBV	394	485	0.18%	0.021%
16	5.660	477	480	482	rBV	626	746	0.28%	0.032%
17	5.748	493	495	499	rBV	502	747	0.28%	0.032%
18	6.242	576	579	580	rBV	412	465	0.17%	0.020%
19	6.389	601	604	605	rVB	628	545	0.20%	0.023%
20	6.412	605	608	611	rBV	355	496	0.18%	0.021%
21	6.706	655	658	660	rBV	403	495	0.18%	0.021%
22	7.282	749	756	765	rBB	27400	47913	17.78%	2.054%
23	7.452	779	785	794	rBB	23995	39587	14.69%	1.697%
24	7.658	813	820	828	rBV	30727	51799	19.22%	2.220%
25	8.134	894	901	910	rVB	60483	101809	37.77%	4.364%
26	8.692	992	996	999	rBB	518	666	0.25%	0.029%
27	8.827	1014	1019	1027	rBB2	27544	46324	17.19%	1.986%
28	9.297	1092	1099	1106	rVB	32455	58056	21.54%	2.488%
29	9.673	1160	1163	1166	rBB	606	595	0.22%	0.026%
30	10.014	1216	1221	1228	rBB	22029	38300	14.21%	1.642%
31	10.555	1306	1313	1321	rBB	34259	58138	21.57%	2.492%
32	10.942	1371	1379	1387	rBB	89312	156972	58.24%	6.728%
33	11.078	1396	1402	1410	rBV2	5539	9722	3.61%	0.417%
34	13.105	1742	1747	1749	rBB2	610	921	0.34%	0.039%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
 Data File : BG021390.D
 Acq On : 9 Mar 2016 6:21
 Operator : UM/SJ
 Sample : H1625-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

35	13.340	1782	1787	1791	rBB	1543	1867	0.69%	0.080%
36	13.551	1820	1823	1825	rBV	1210	1145	0.42%	0.049%
37	13.580	1825	1828	1831	rVB	4132	3817	1.42%	0.164%
38	13.616	1831	1834	1840	rBB	2061	2835	1.05%	0.122%
39	13.904	1880	1883	1886	rBB	1860	1921	0.71%	0.082%
40	13.945	1888	1890	1892	rBB	808	556	0.21%	0.024%
41	14.139	1918	1923	1927	rBV	59818	81276	30.16%	3.484%
42	14.186	1927	1931	1936	rVB	26903	37461	13.90%	1.606%
43	14.239	1937	1940	1943	rBB	845	895	0.33%	0.038%
44	14.385	1961	1965	1967	rBB	529	588	0.22%	0.025%
45	14.438	1967	1974	1981	rBB	80573	126325	46.87%	5.414%
46	14.562	1990	1995	1999	rBV2	9153	13168	4.89%	0.564%
47	14.615	1999	2004	2008	rVV2	6894	8984	3.33%	0.385%
48	14.685	2013	2016	2017	rBV2	645	596	0.22%	0.026%
49	14.744	2019	2026	2033	rVB2	127613	204685	75.94%	8.773%
50	14.820	2033	2039	2042	rBB2	2663	3206	1.19%	0.137%
51	14.932	2053	2058	2070	rBV3	8952	16056	5.96%	0.688%
52	15.055	2074	2079	2080	rBV2	1714	2664	0.99%	0.114%
53	15.085	2083	2084	2086	rVV	1316	1227	0.46%	0.053%
54	15.108	2086	2088	2091	rVV3	1939	2568	0.95%	0.110%
55	15.143	2091	2094	2101	rVB3	3041	5532	2.05%	0.237%
56	15.231	2101	2109	2114	rBV3	2620	4940	1.83%	0.212%
57	15.296	2116	2120	2124	rBV3	1793	2569	0.95%	0.110%
58	15.455	2146	2147	2151	rVV2	888	920	0.34%	0.039%
59	15.519	2154	2158	2160	rBV3	1734	2750	1.02%	0.118%
60	15.561	2160	2165	2170	rVB	13380	18577	6.89%	0.796%
61	15.619	2170	2175	2179	rBV4	1817	3584	1.33%	0.154%
62	15.655	2179	2181	2183	rVV2	626	562	0.21%	0.024%
63	15.684	2184	2186	2188	rVB2	1426	836	0.31%	0.036%
64	15.731	2188	2194	2201	rBV	104284	157537	58.45%	6.752%
65	15.848	2209	2214	2219	rVB4	2134	4112	1.53%	0.176%
66	15.960	2225	2233	2239	rBV5	6390	14818	5.50%	0.635%
67	16.007	2239	2241	2243	rVB2	1039	758	0.28%	0.032%
68	16.025	2243	2244	2246	rBV2	1286	850	0.32%	0.036%
69	16.054	2246	2249	2253	rVB4	1590	1779	0.66%	0.076%
70	16.113	2257	2259	2262	rBV2	2241	2674	0.99%	0.115%
71	16.183	2268	2271	2274	rVB3	2799	3472	1.29%	0.149%

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
 Data File : BG021390.D
 Acq On : 9 Mar 2016 6:21
 Operator : UM/SJ
 Sample : H1625-15
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 JHFH2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
 Title : SVOA CALIBRATION

72	16.219	2274	2277	2278	rBV3	1037	588	0.22%	0.025%
73	16.266	2284	2285	2289	rVB3	1373	1194	0.44%	0.051%
74	16.342	2297	2298	2300	rBV2	1187	822	0.30%	0.035%
75	16.418	2306	2311	2313	rBV	16181	21413	7.94%	0.918%
76	16.518	2326	2328	2332	rVB4	2679	3518	1.31%	0.151%
77	16.553	2332	2334	2335	rBV2	1141	594	0.22%	0.025%
78	16.595	2339	2341	2342	rBV	1537	1237	0.46%	0.053%
79	16.636	2347	2348	2352	rVB3	1269	947	0.35%	0.041%
80	16.689	2352	2357	2359	rBV4	1122	1717	0.64%	0.074%
81	16.759	2362	2369	2373	rBV5	2384	6541	2.43%	0.280%
82	16.794	2373	2375	2376	rBV2	977	931	0.35%	0.040%
83	16.871	2386	2388	2389	rBV2	1135	867	0.32%	0.037%
84	16.924	2394	2397	2401	rBV5	2151	4092	1.52%	0.175%
85	16.988	2404	2408	2410	rBV4	2300	2118	0.79%	0.091%
86	17.006	2410	2411	2413	rBV2	1621	1039	0.39%	0.045%
87	17.206	2441	2445	2449	rBV	9251	13170	4.89%	0.564%
88	17.264	2450	2455	2459	rVB4	7596	11587	4.30%	0.497%
89	17.347	2467	2469	2471	rBV3	1801	1571	0.58%	0.067%
90	17.482	2485	2492	2500	rBV	156546	230982	85.70%	9.900%
91	17.582	2503	2509	2515	rVB2	105806	161324	59.86%	6.915%
92	17.646	2519	2520	2521	rBV	1633	846	0.31%	0.036%
93	17.805	2545	2547	2548	rBV2	1903	1650	0.61%	0.071%
94	17.946	2568	2571	2576	rVB2	8001	9310	3.45%	0.399%
95	18.122	2599	2601	2607	rBV6	2502	4256	1.58%	0.182%
96	18.334	2635	2637	2640	rBV3	3235	3851	1.43%	0.165%
97	18.486	2661	2663	2664	rBV2	3303	2369	0.88%	0.102%
98	18.633	2685	2688	2691	rBV5	5127	6188	2.30%	0.265%
99	19.855	2891	2896	2903	rVB	125348	173742	64.46%	7.447%
100	21.747	3213	3218	3224	rVB	162304	269521	100.00%	11.552%


Sum of corrected areas: 2333092

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021390.D
Acq On : 9 Mar 2016 6:21
Operator : UM/SJ
Sample : H1625-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampled :
JHFH2

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

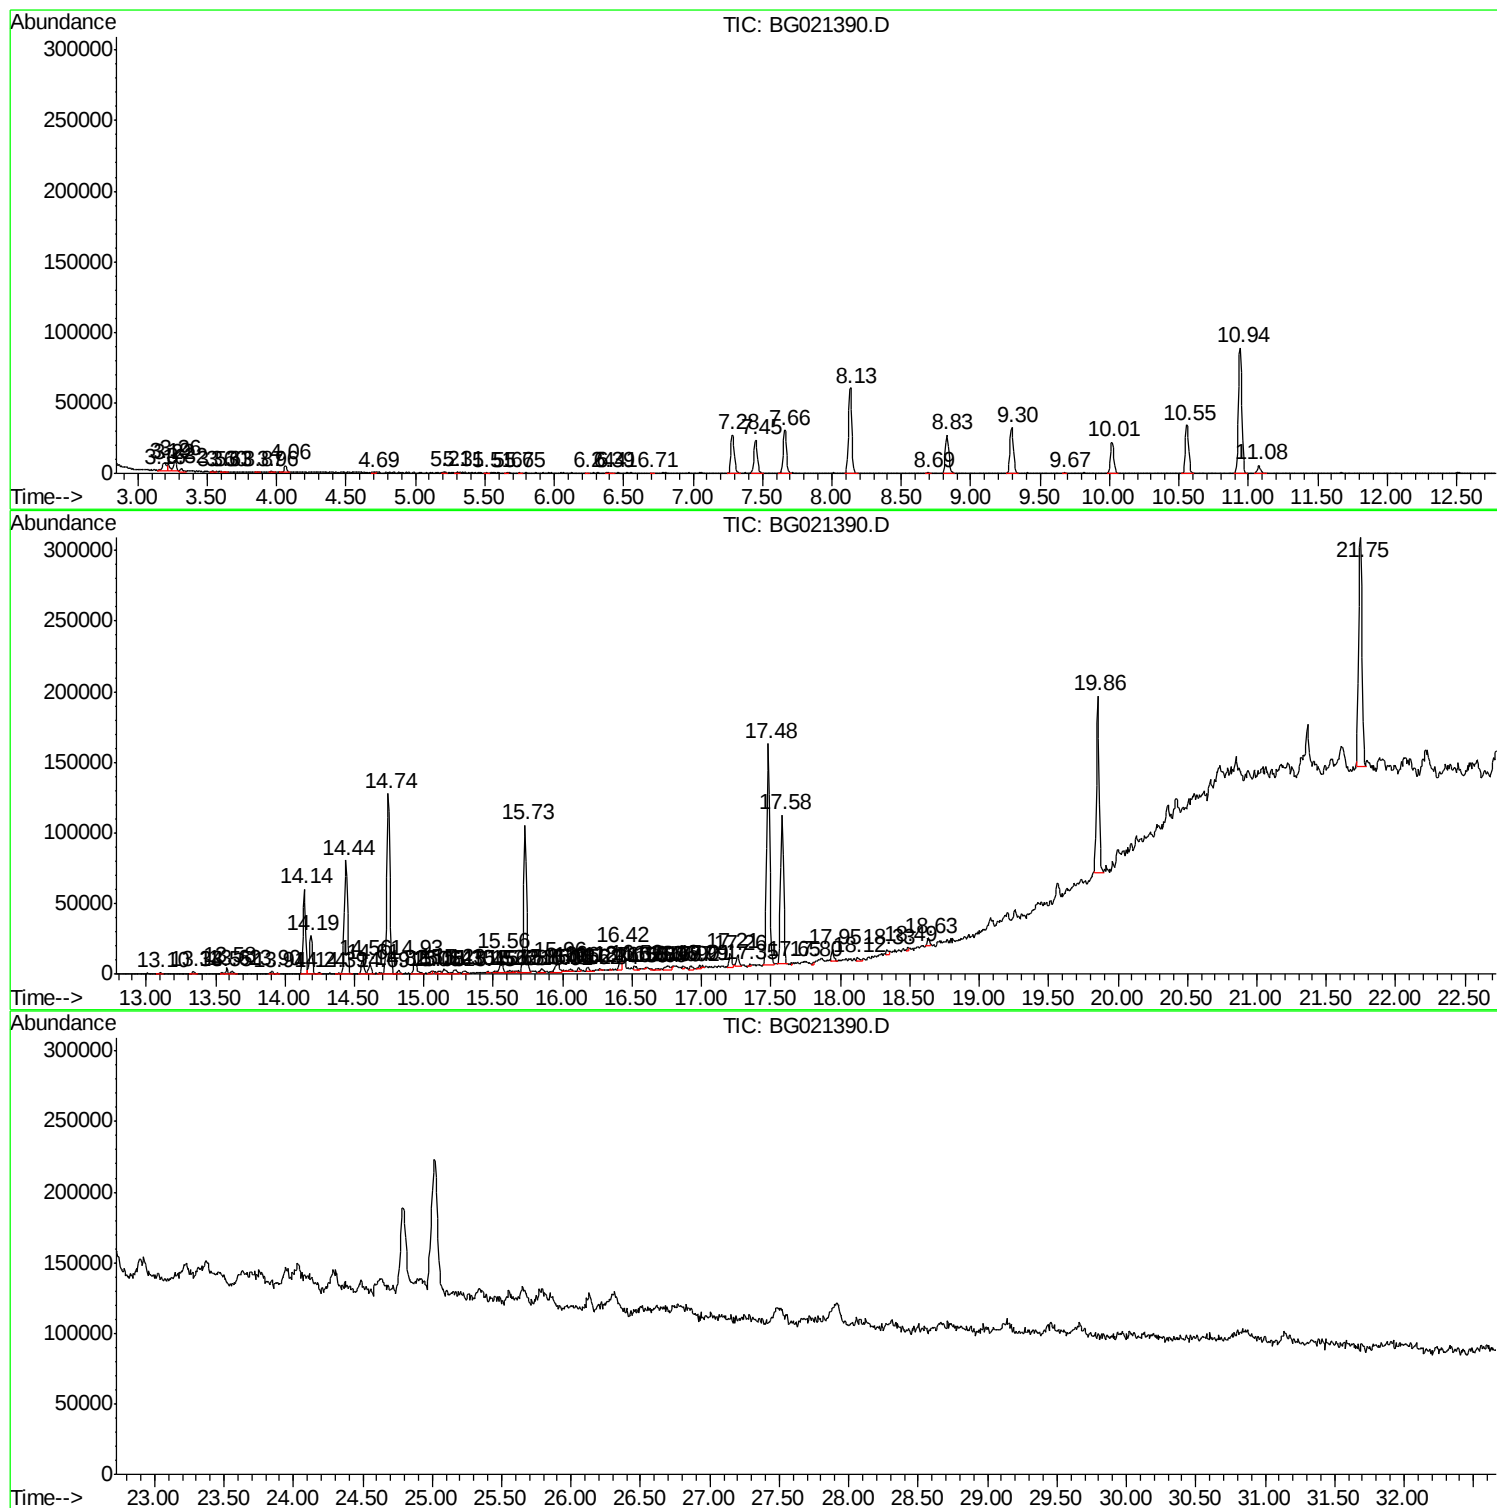

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021390.D
Acq On : 9 Mar 2016 6:21
Operator : UM/SJ
Sample : H1625-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH2

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_G\Data\BG030816\
Data File : BG021390.D
Acq On : 9 Mar 2016 6:21
Operator : UM/SJ
Sample : H1625-15
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
JHFH2

Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG030316.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc