

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030817\
 Data File : BG026131.D
 Acq On : 9 Mar 2017 2:52
 Operator : SJ/MA
 Sample : I2062-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AD0

Quant Time: Mar 15 16:28:46 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 15 16:21:45 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	163175	20.00	ng/ul	0.00
2) Naphthalene-d8	10.87	136	720226	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.67	164	423495	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.39	188	1024639	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	1216626	20.00	ng/ul	0.00
23) Perylene-d12	24.83	264	1204130	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.48	165	211008	19.78	ng/uL	0.00
7) Acenaphthylene-d8	14.36	160	913697	25.30	ng/ul	0.00
10) Fluorene-d10	15.66	176	683608	25.95	ng/ul	0.00
15) Anthracene-d10	17.49	188	1070345	23.51	ng/ul	0.00
19) Pyrene-d10	19.77	212	1331428	21.45	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.62	264	1315342	25.33	ng/ul	0.00
Target Compounds						
17) Fluoranthene	19.44	202	82436	1.46	ng/ul	Qvalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030817\
Data File : BG026131.D
Acq On : 9 Mar 2017 2:52
Operator : SJ/MA
Sample : I2062-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AD0

Quant Time: Mar 15 16:28:46 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 15 16:21:45 2017
Response via : Initial Calibration

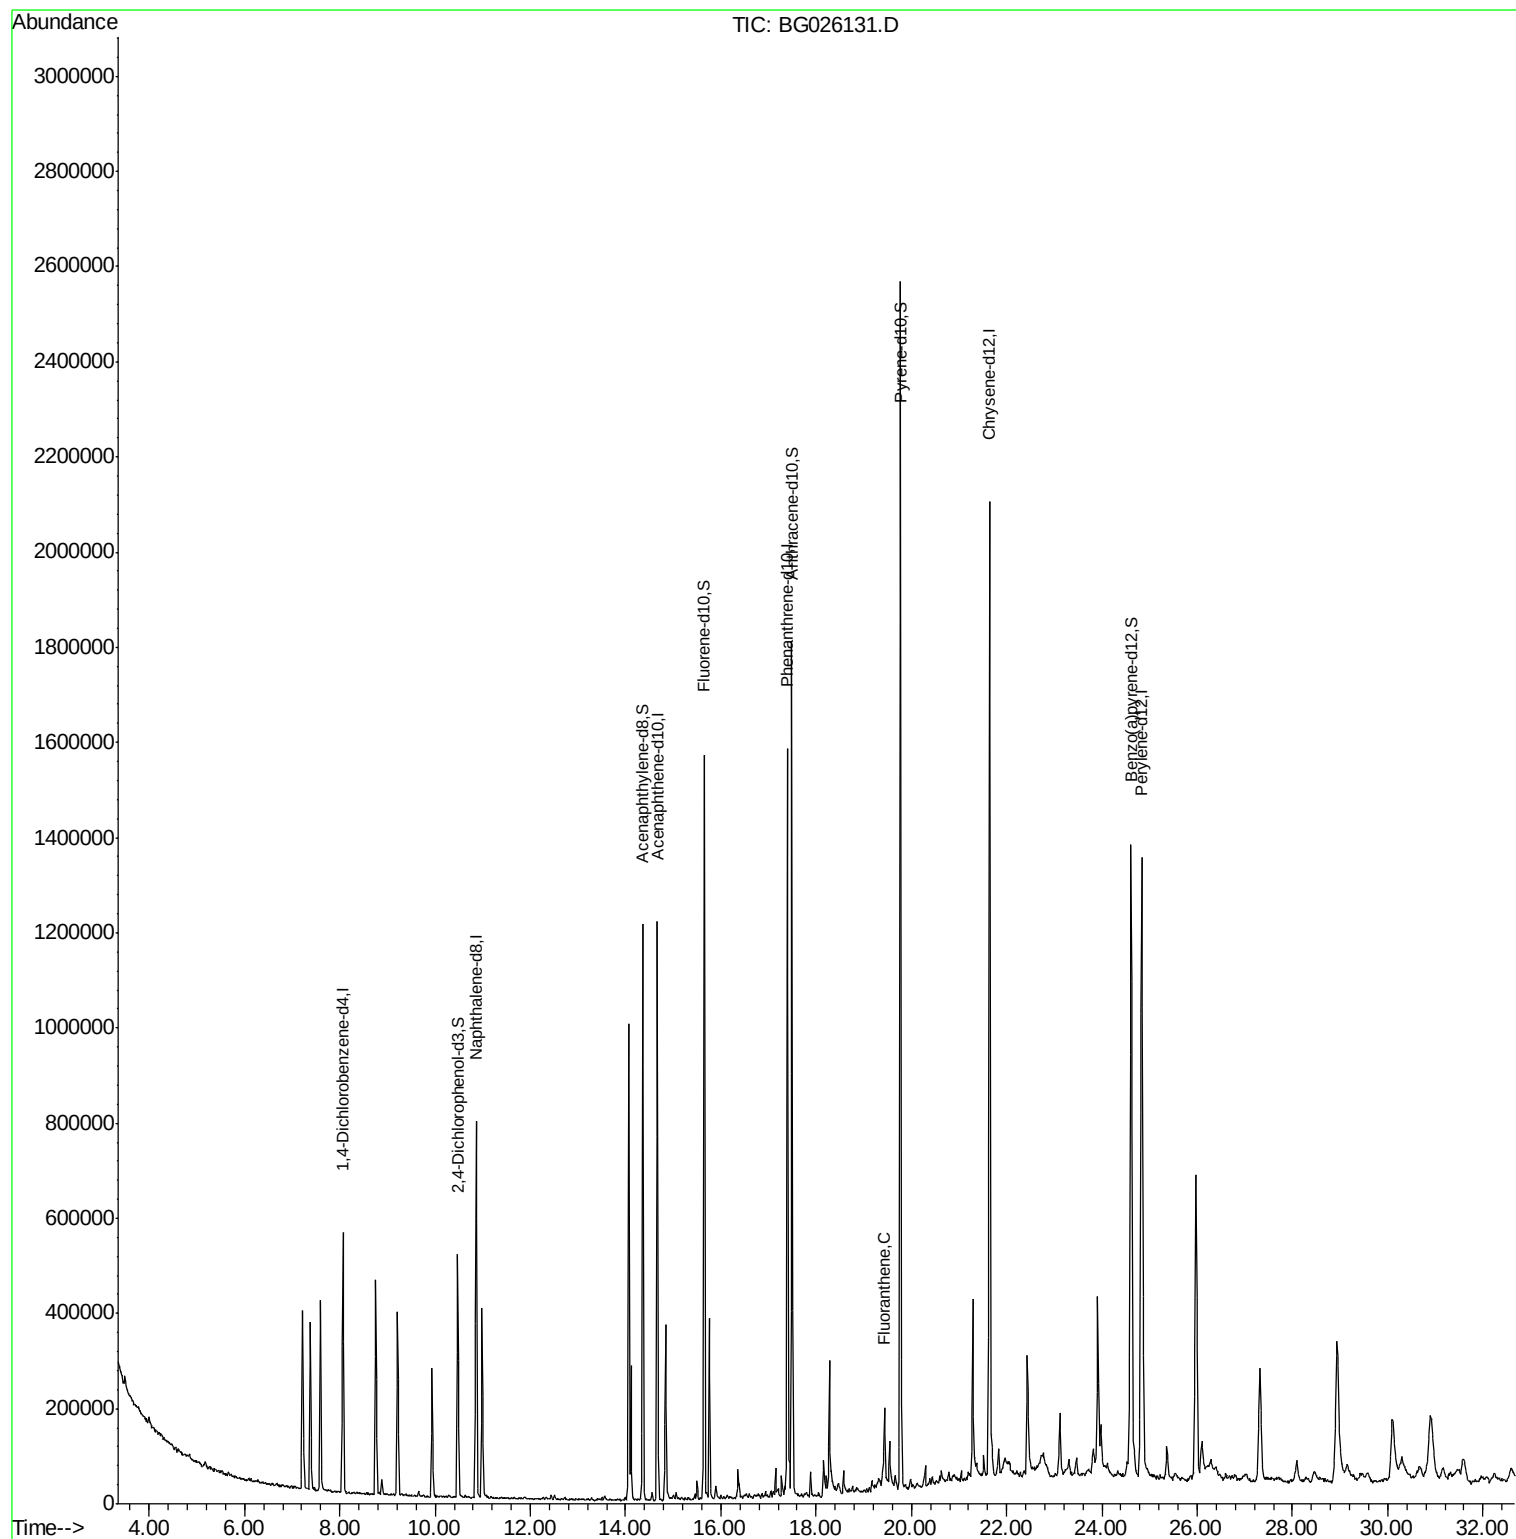


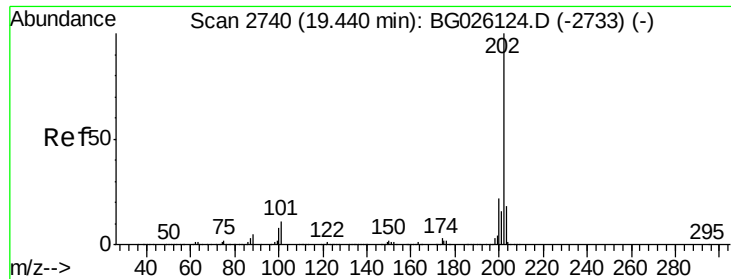

#17
 Fluoranthene
 Concen: 1.46 ng/ul
 RT: 19.44 min Scan# 2740
 Delta R.T. 0.00 min
 Lab File: BG026131.D
 Acq: 9 Mar 2017 2:52

Instrument :
 BNA_G
 ClientSampleId :
 C0AD0

Tgt Ion	Ratio	Lower	Upper
202	100		
101	10.7	9.8	14.8
100	8.6	7.5	11.3

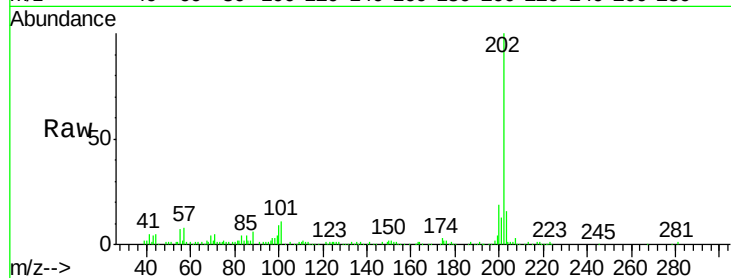

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

