
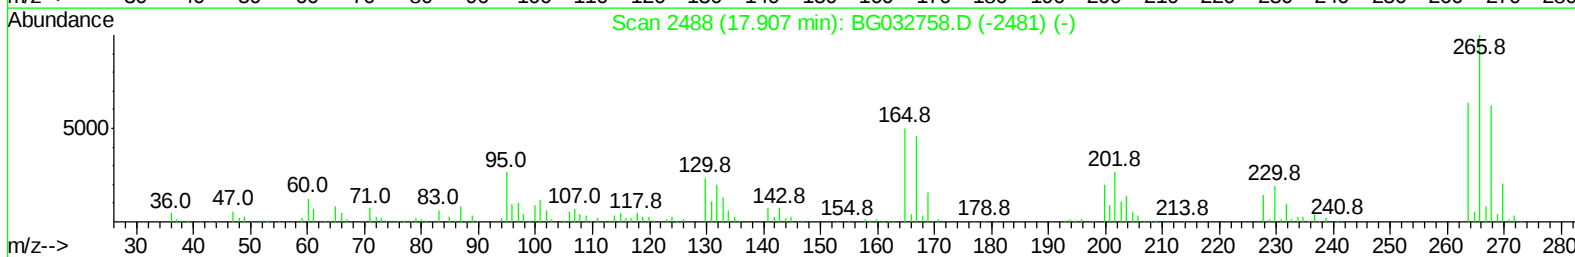
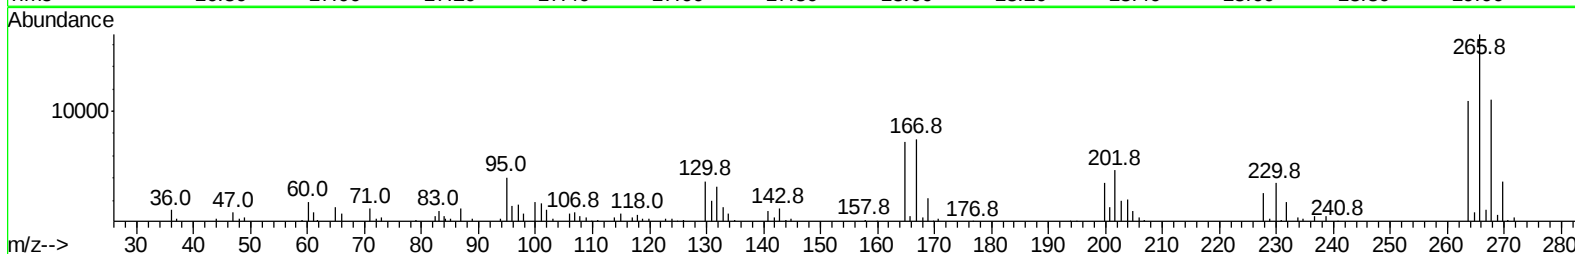


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030818\
Data File : BG033037.D
Acq On : 8 Mar 2018 12:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 02:58:35 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 17:38:59 2018
Response via : Initial Calibration

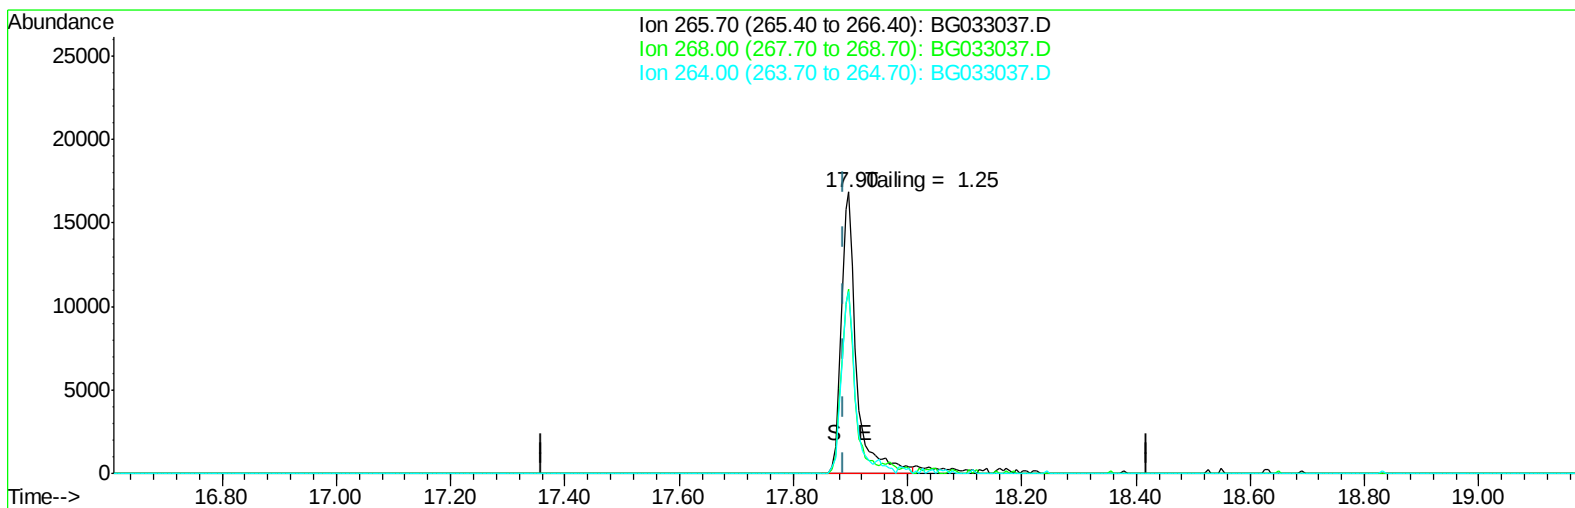

TIC: BG033037.D

(69) Pentachlorophenol (C)




17.897min (+0.008) 80022.28ng

response 31102

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	65.28
264.00	62.00	64.55
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030818\
Data File : BG033037.D
Acq On : 8 Mar 2018 12:36
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 02:58:35 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 17:38:59 2018
Response via : Initial Calibration

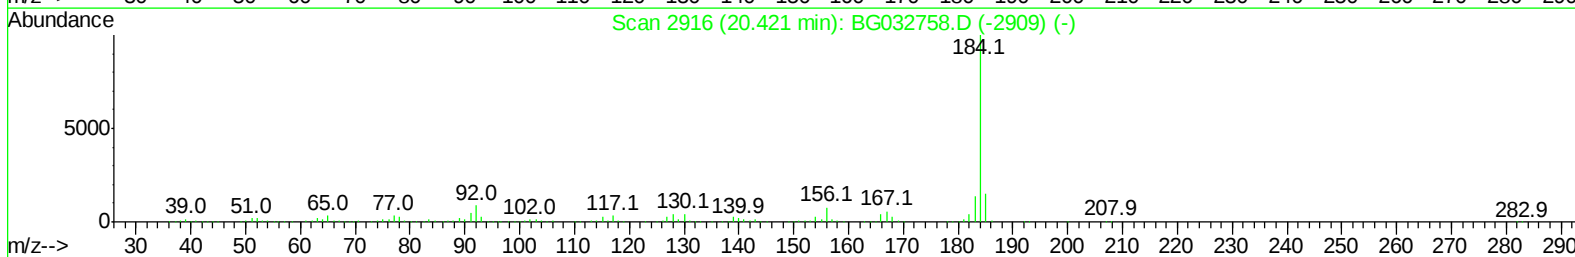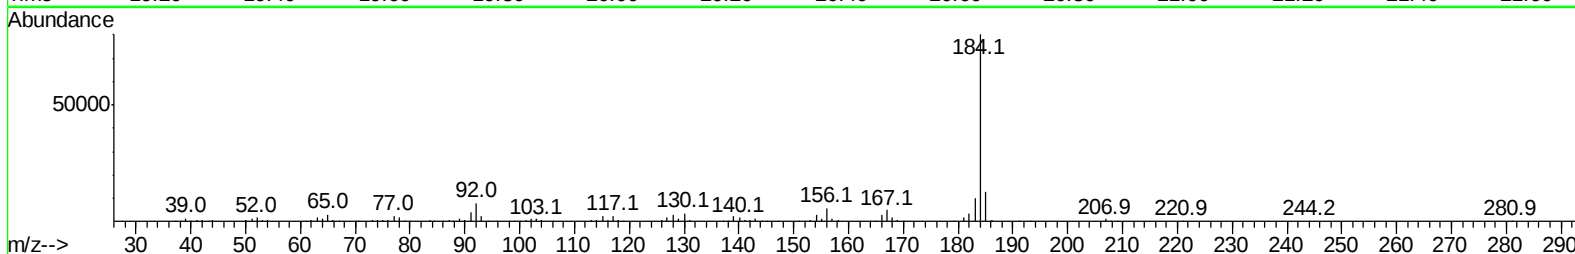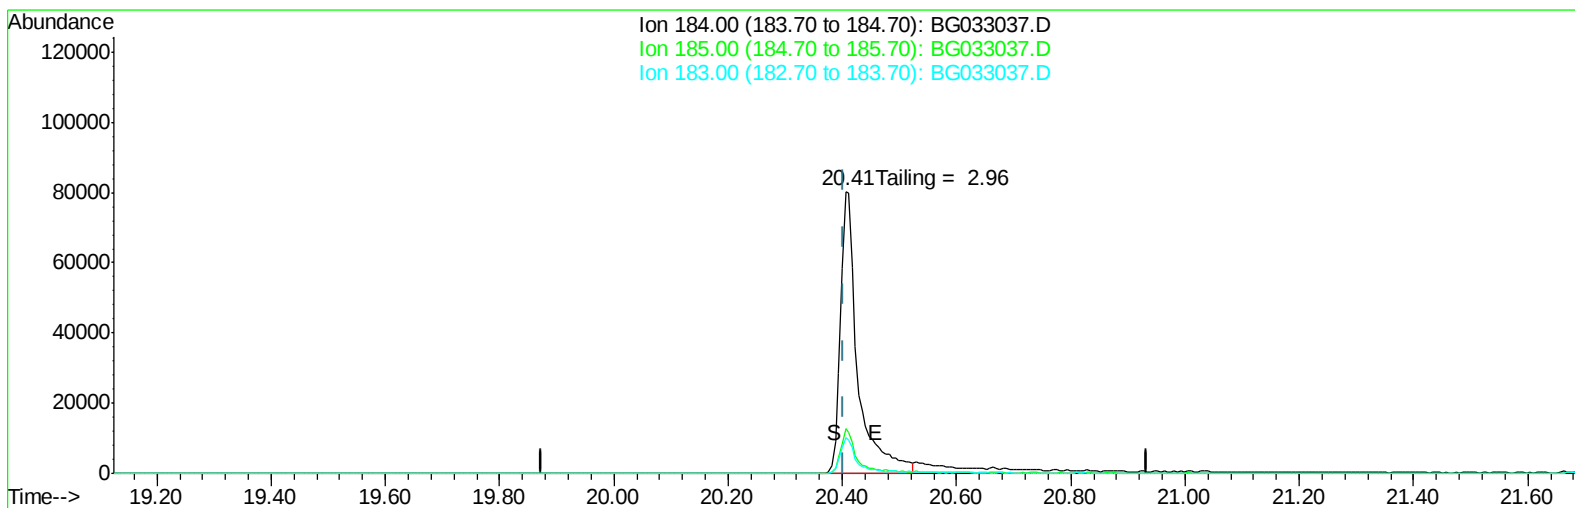

TIC: BG033037.D

(76) Benzidine

20.405min (+0.002) 0.00ng

response 171017

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.99
183.00	13.30	12.80
0.00	0.00	0.00