
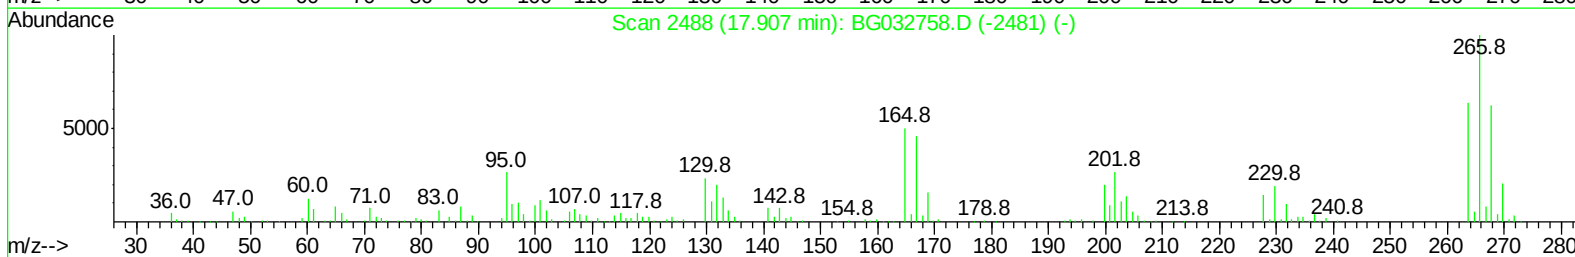
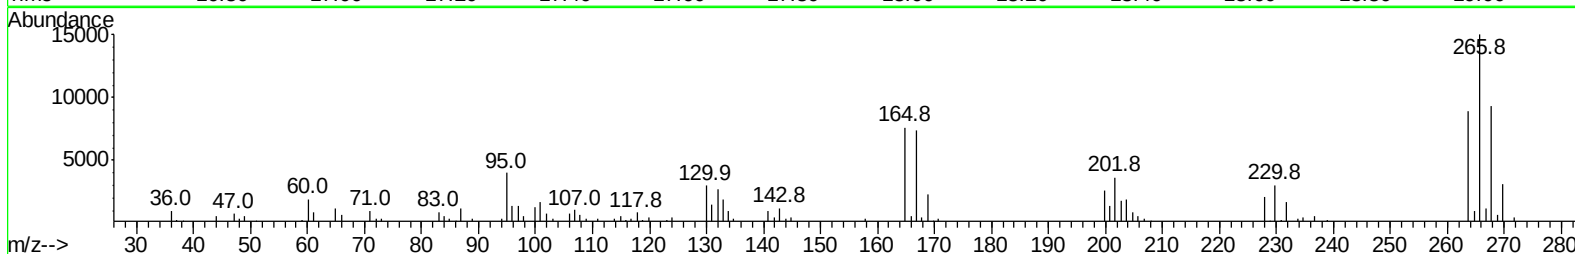


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030818\
Data File : BG033055.D
Acq On : 9 Mar 2018 00:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 03:00:06 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 17:38:59 2018
Response via : Initial Calibration

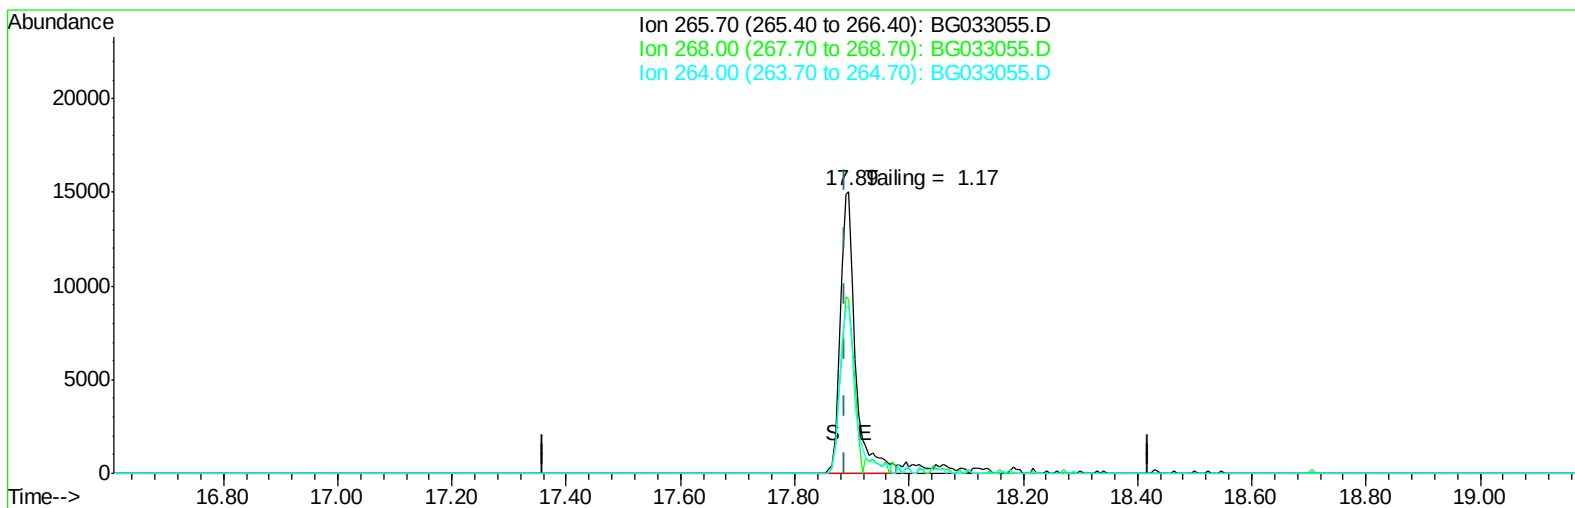

TIC: BG033055.D

(69) Pentachlorophenol (C)




17.894min (+0.005) 16201.05ng

response 27636

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.92
264.00	62.00	59.58
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030818\
Data File : BG033055.D
Acq On : 9 Mar 2018 00:47
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 09 03:00:06 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 06 17:38:59 2018
Response via : Initial Calibration

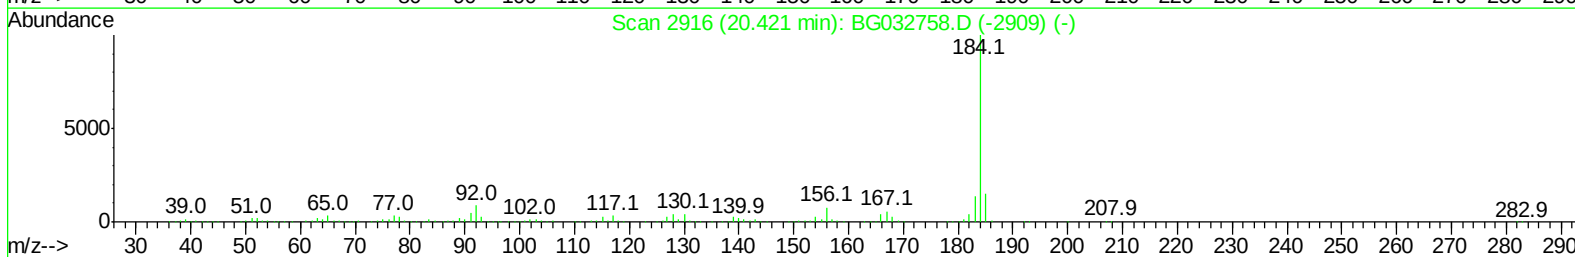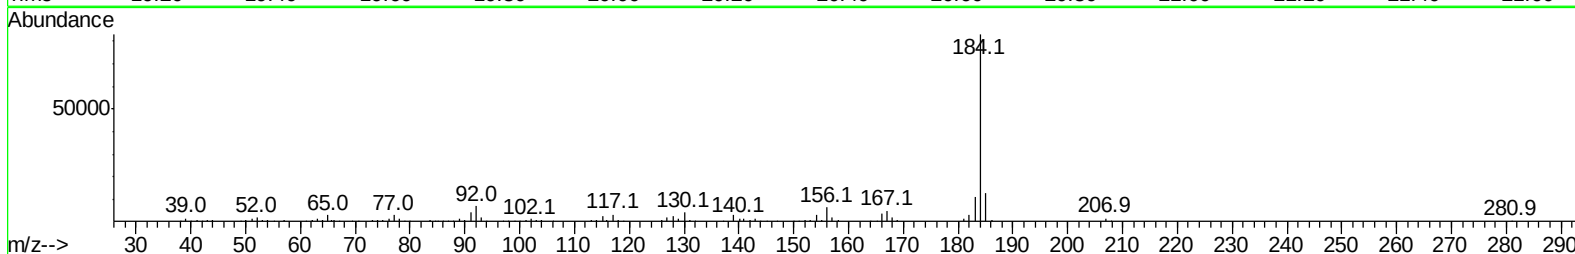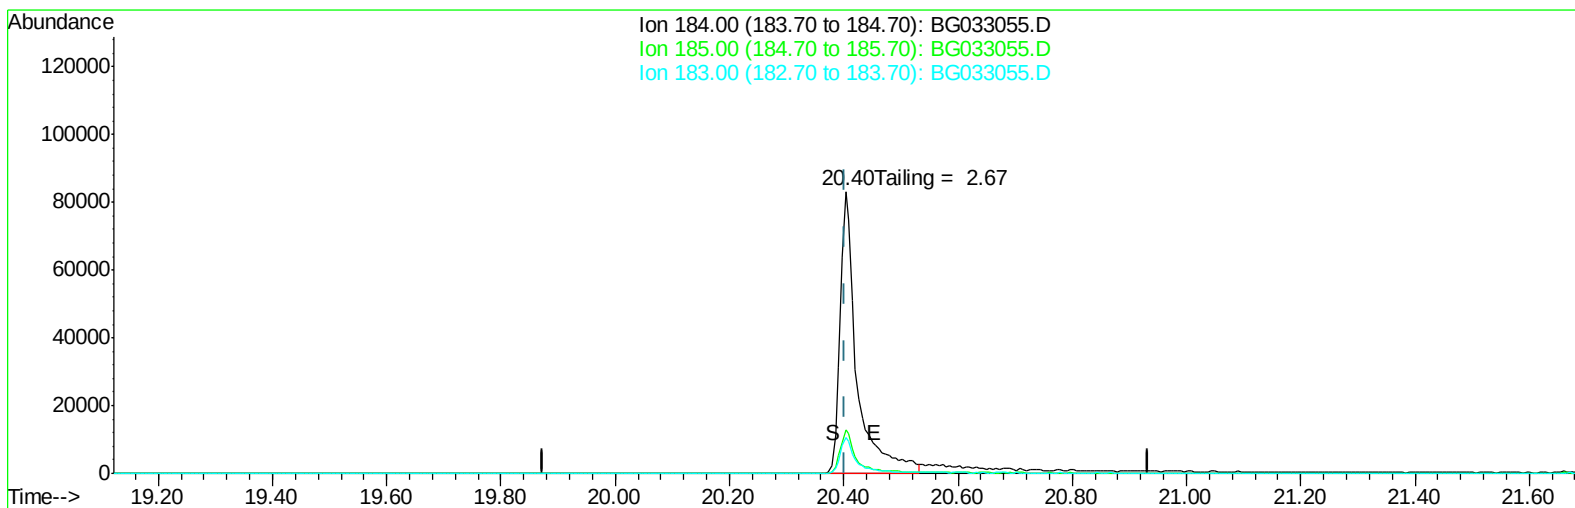

TIC: BG033055.D

(76) Benzidine

20.403min (-0.001) 0.00ng

response 171227

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.36
183.00	13.30	12.89
0.00	0.00	0.00