


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030818\
 Data File : BG033037.D
 Acq On : 8 Mar 2018 12:36
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 06 17:38:59 2018

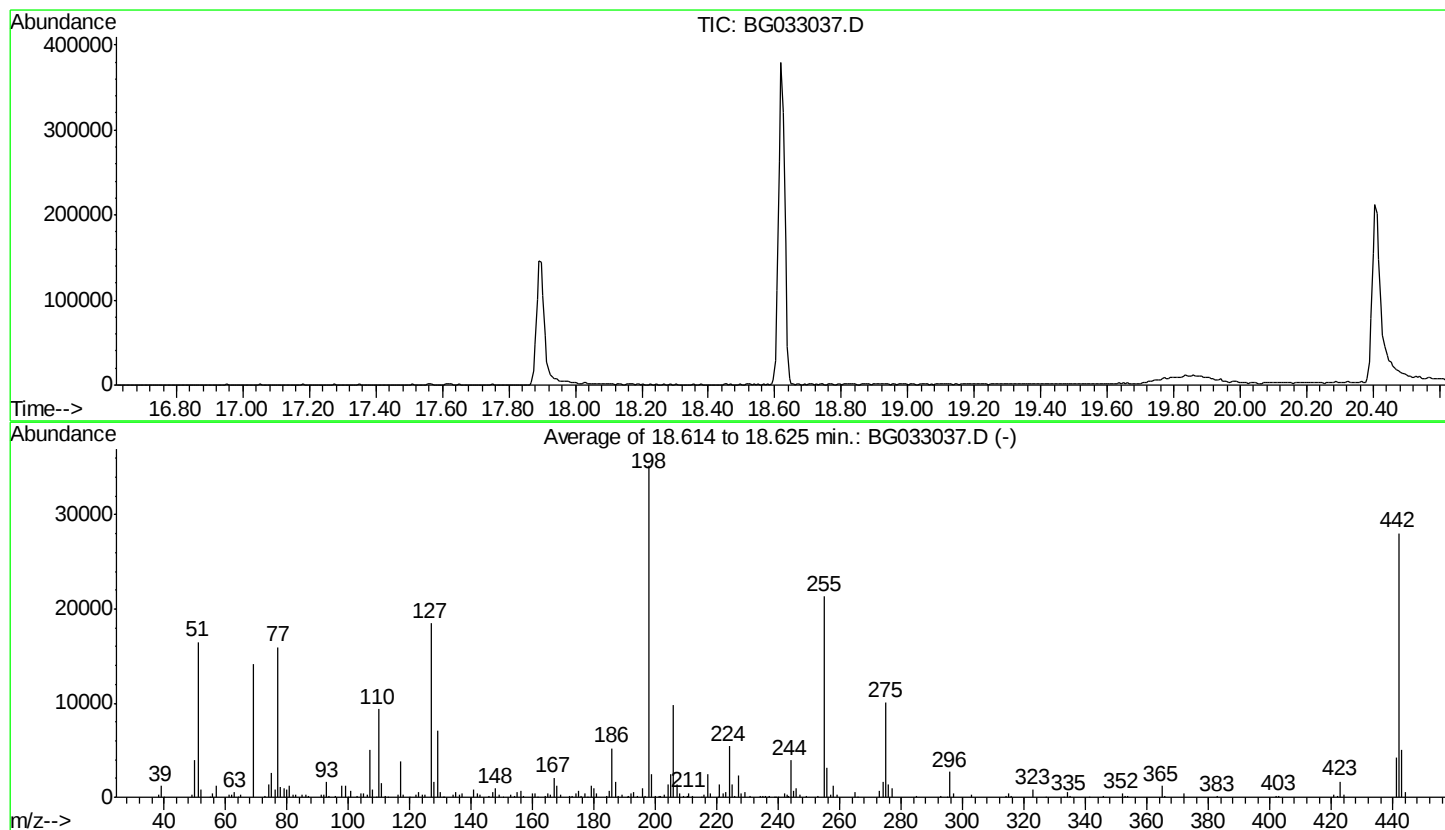

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	16466	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.1	14140	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.4	18448	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	35232	PASS
199	198	5	9	6.9	2444	PASS
275	198	10	60	28.4	10005	PASS
365	198	1	100	3.4	1191	PASS
441	442	0.01	24	15.0	4216	PASS
442	198	50	100	79.5	28026	PASS
443	442	15	24	18.0	5054	PASS