


Data Path : Z:\HPCHEM1\BNA G\DATA\BG030818\
 Data File : BG033055.D
 Acq On : 9 Mar 2018 00:47
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 06 17:38:59 2018

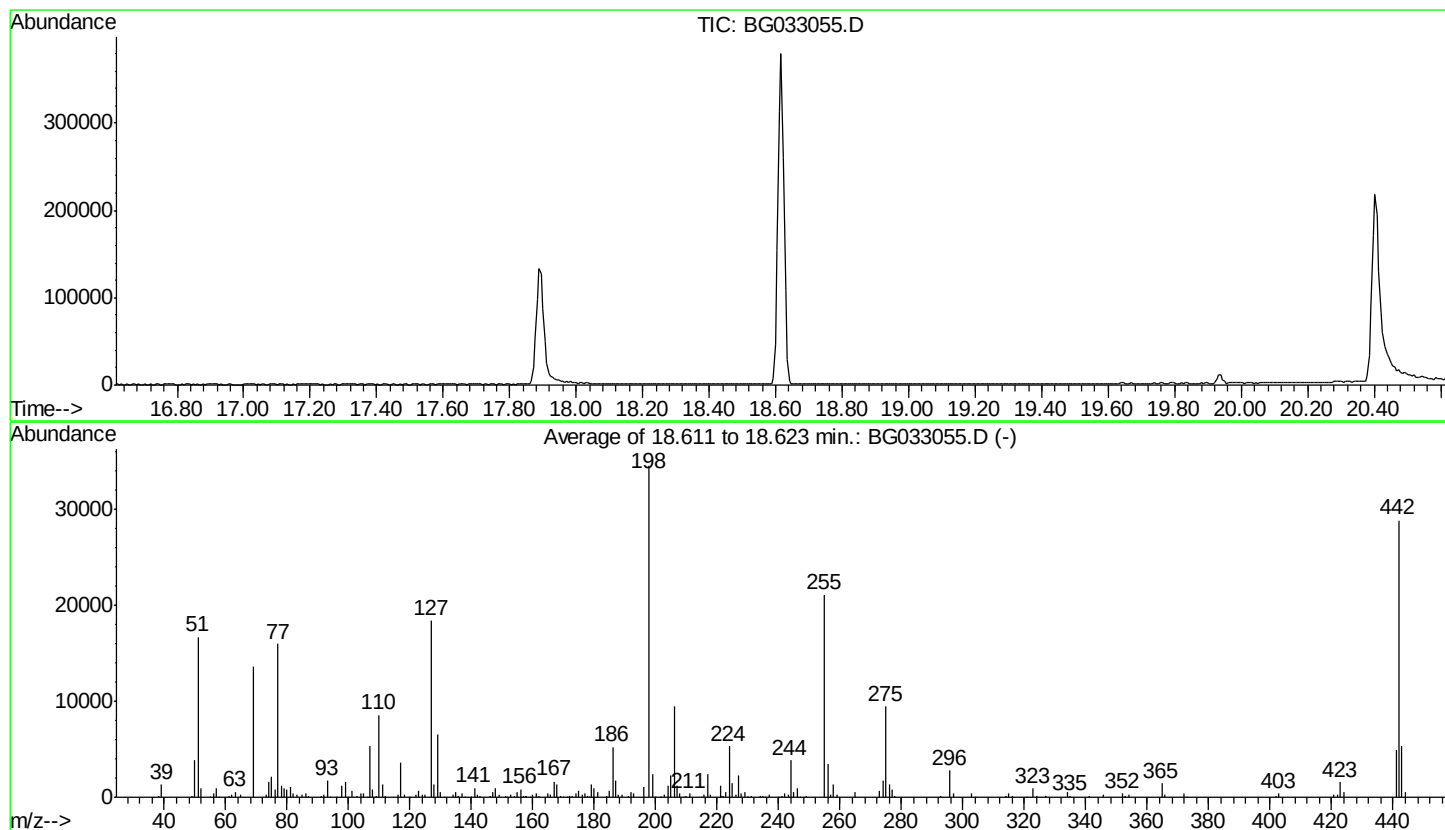

AutoFind: Scans 2608, 2609, 2610; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.4	16698	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	39.3	13543	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.1	18322	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34482	PASS
199	198	5	9	6.9	2384	PASS
275	198	10	60	27.4	9442	PASS
365	198	1	100	4.2	1463	PASS
441	442	0.01	24	17.2	4958	PASS
442	198	50	100	83.5	28778	PASS
443	442	15	24	18.7	5370	PASS