

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030917\
 Data File : BG026160.D
 Acq On : 9 Mar 2017 21:54
 Operator : SJ/MA
 Sample : I2069-18
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ3

Quant Time: Mar 16 03:08:59 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 15 15:39:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	105460	20.00	ng/ul	0.00
2) Naphthalene-d8	10.86	136	473951	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.67	164	289997	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.40	188	719203	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	780310	20.00	ng/ul	0.00
23) Perylene-d12	24.84	264	752334	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.48	165	180153	25.66	ng/uL	0.00
7) Acenaphthylene-d8	14.36	160	820324	33.18	ng/ul	0.00
10) Fluorene-d10	15.65	176	611272	33.89	ng/ul	0.00
15) Anthracene-d10	17.49	188	931018	29.13	ng/ul	0.00
19) Pyrene-d10	19.77	212	1106718	27.79	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.61	264	1042890	32.14	ng/ul	0.00
Target Compounds				Qvalue		
17) Fluoranthene	19.44	202	59406	1.50	ng/ul#	96
20) Pyrene	19.80	202	56866	1.14	ng/ul	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG030917\
Data File : BG026160.D
Acq On : 9 Mar 2017 21:54
Operator : SJ/MA
Sample : I2069-18
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AJ3

Quant Time: Mar 16 03:08:59 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 15 15:39:02 2017
Response via : Initial Calibration




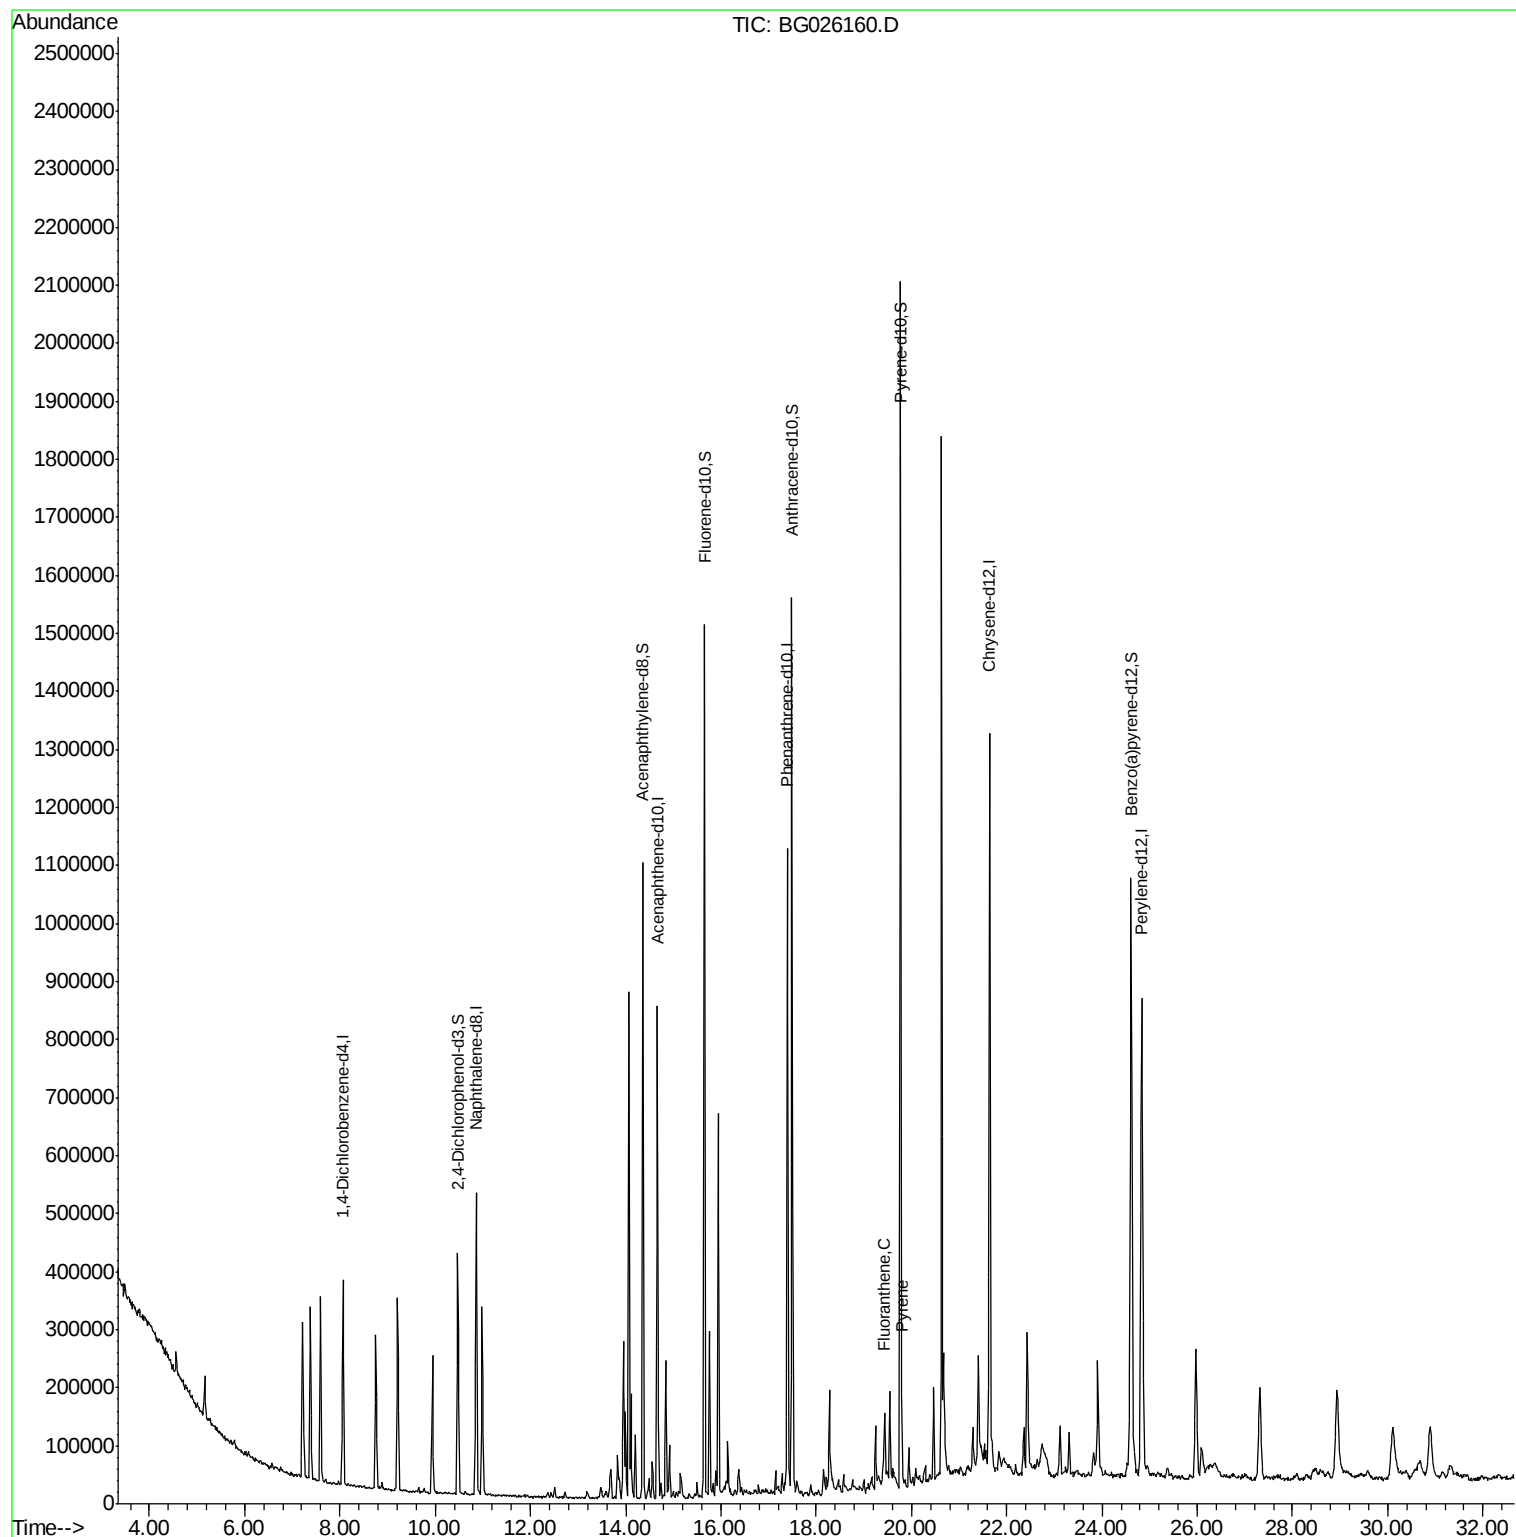


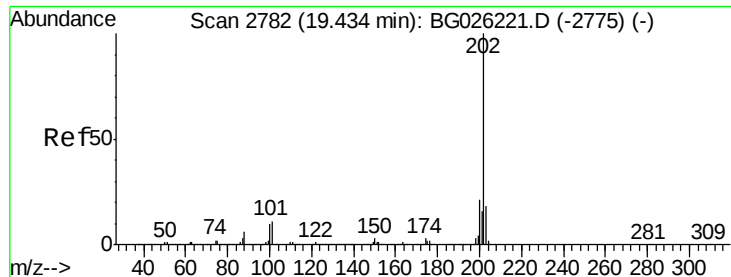

#17
Fluoranthene
 Concen: 1.50 ng/ul
 RT: 19.44 min Scan# 2740
 Delta R.T. -0.00 min
 Lab File: BG026160.D
 Acq: 9 Mar 2017 21:54

Instrument :
 BNA_G
 ClientSampled :
 C0AJ3

Tot Ion	Ratio	Lower	Upper
202	100		
101	13.3	9.8	14.8
100	11.3	7.5	11.3#

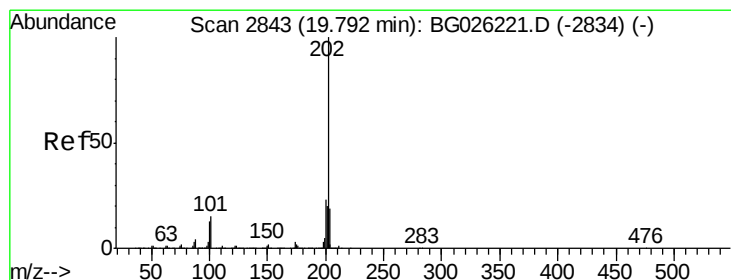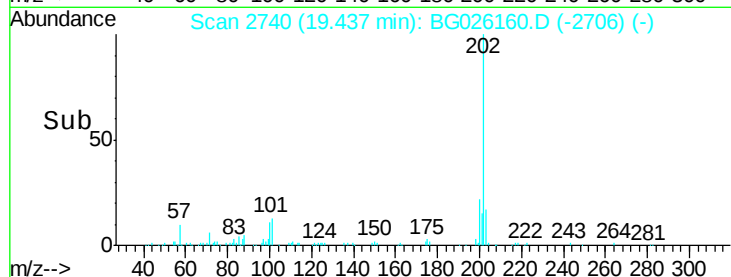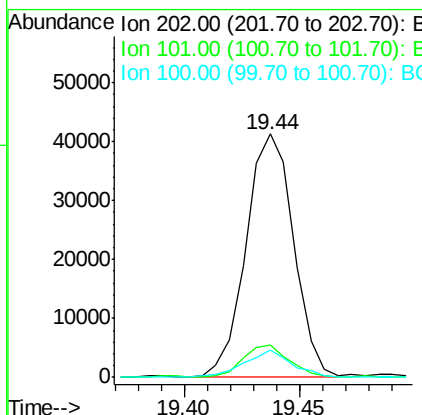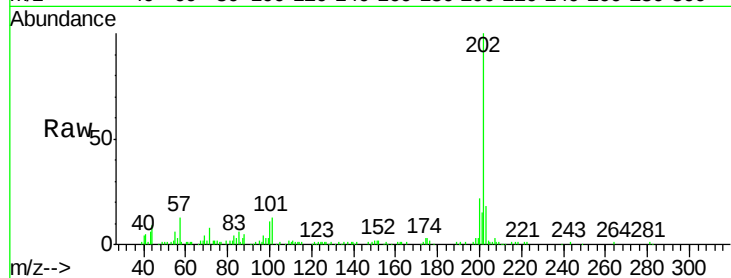

#20
Pyrene
 Concen: 1.14 ng/ul
 RT: 19.80 min Scan# 2802
 Delta R.T. 0.00 min
 Lab File: BG026160.D
 Acq: 9 Mar 2017 21:54

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.5	11.2	16.8
100	10.2	9.8	14.6

