

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030917\
 Data File : BG026161.D
 Acq On : 9 Mar 2017 22:34
 Operator : SJ/MA
 Sample : I2069-20
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ5

Quant Time: Mar 15 15:49:07 2017
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Mar 15 15:39:02 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	110982	20.00	ng/ul	0.00
2) Naphthalene-d8	10.86	136	491495	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.67	164	301018	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.40	188	753212	20.00	ng/ul	0.00
18) Chrysene-d12	21.64	240	804085	20.00	ng/ul	0.00
23) Perylene-d12	24.83	264	775458	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.48	165	122361	16.81	ng/uL	0.00
7) Acenaphthylene-d8	14.36	160	559678	21.81	ng/ul	0.00
10) Fluorene-d10	15.65	176	426958	22.80	ng/ul	0.00
15) Anthracene-d10	17.49	188	672271	20.08	ng/ul	0.00
19) Pyrene-d10	19.77	212	783776	19.10	ng/ul	0.00
26) Benzo(a)pyrene-d12	24.61	264	693572	20.74	ng/ul	0.00
Target Compounds				Qvalue		
17) Fluoranthene	19.44	202	80028	1.93	ng/ul	98
20) Pyrene	19.80	202	73235	1.43	ng/ul#	94
24) Benzo(b)fluoranthene	23.83	252	50637	1.15	ng/ul	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG030917\
Data File : BG026161.D
Acq On : 9 Mar 2017 22:34
Operator : SJ/MA
Sample : I2069-20
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0AJ5

Quant Time: Mar 15 15:49:07 2017
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM-EPA-BG030317-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Mar 15 15:39:02 2017
Response via : Initial Calibration

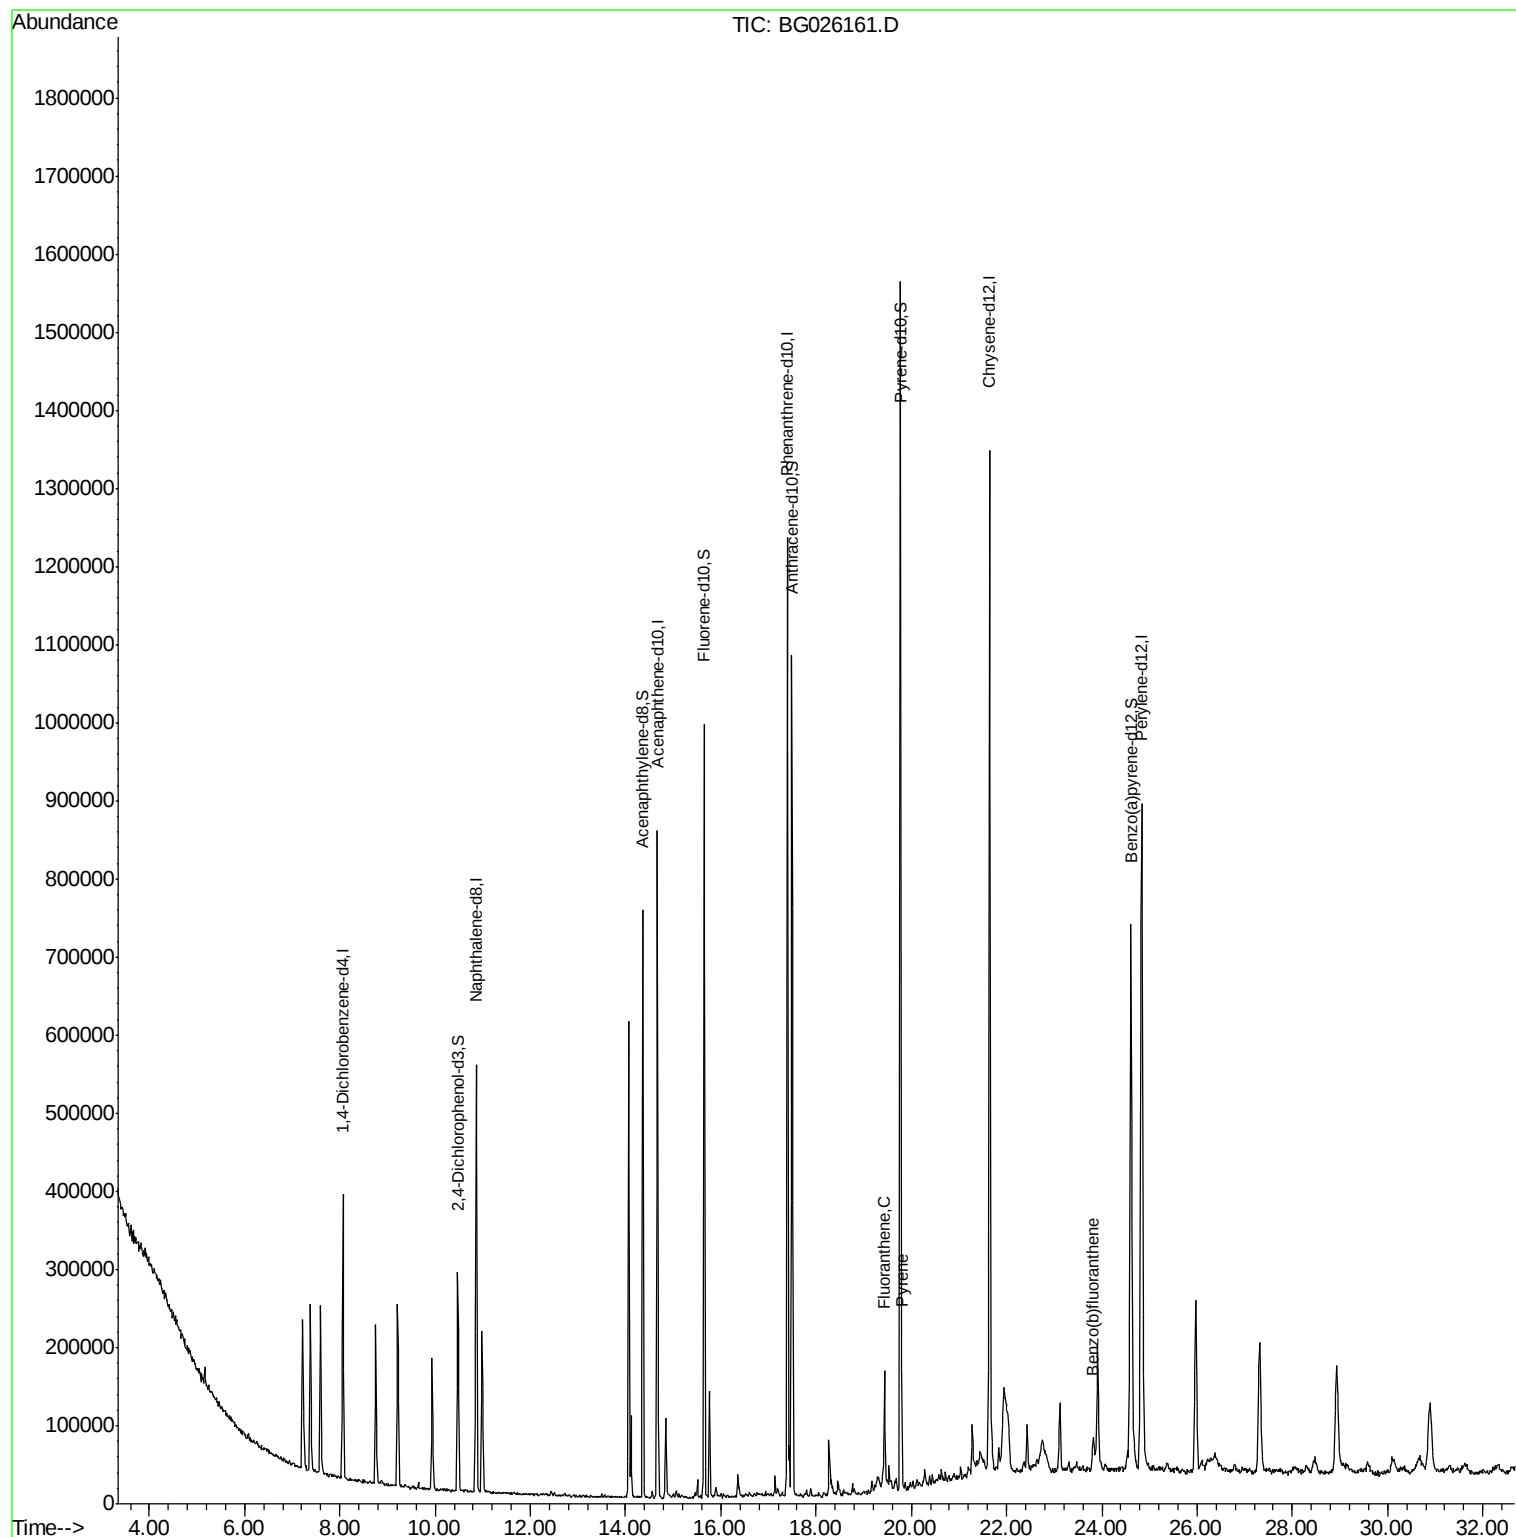


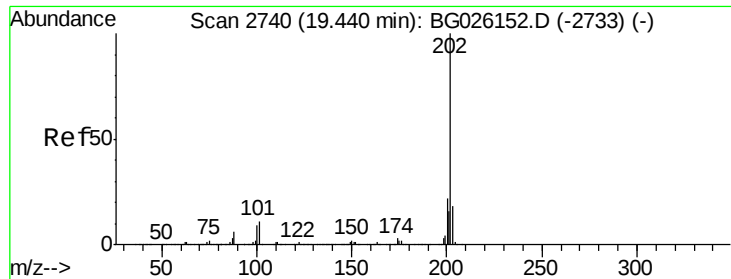




#17
Fluoranthene
 Concen: 1.93 ng/ul
 RT: 19.44 min Scan# 2740
 Delta R.T. -0.00 min
 Lab File: BG026161.D
 Acq: 9 Mar 2017 22:34

Instrument :
 BNA_G
 ClientSampleId :
 C0AJ5

Tgt Ion	Ratio	Lower	Upper
202	100		
101	11.3	9.8	14.8
100	9.9	7.5	11.3

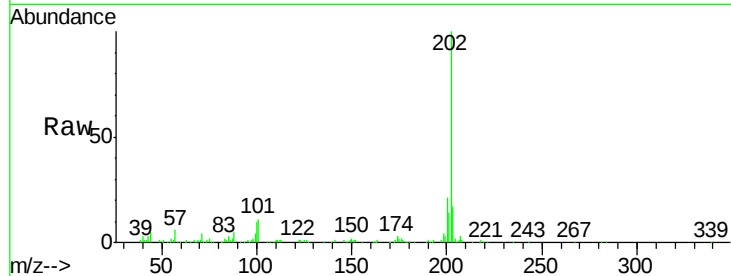


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

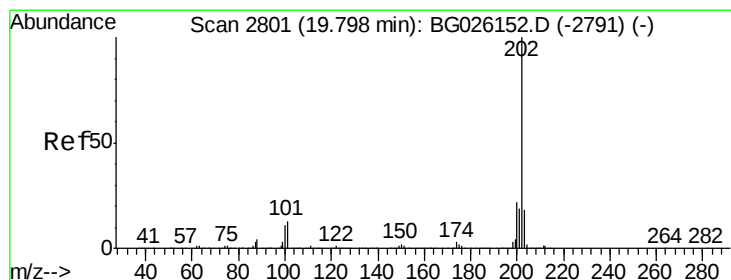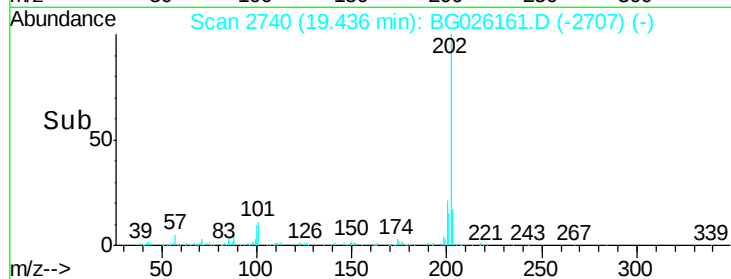
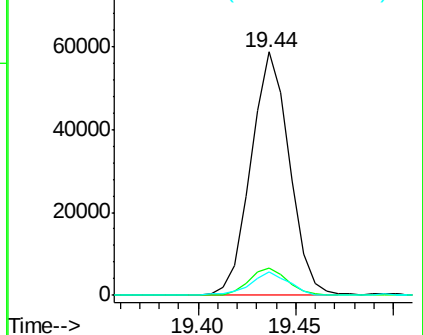



#20
Pyrene
 Concen: 1.43 ng/ul
 RT: 19.80 min Scan# 2802
 Delta R.T. 0.00 min
 Lab File: BG026161.D
 Acq: 9 Mar 2017 22:34

Tgt Ion	Ratio	Lower	Upper
202	100		
101	9.8	11.2	16.8#
100	12.4	9.8	14.6

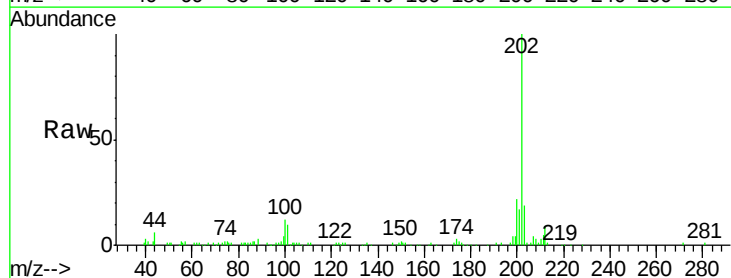

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

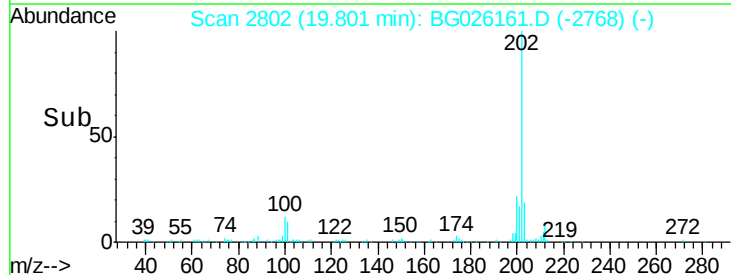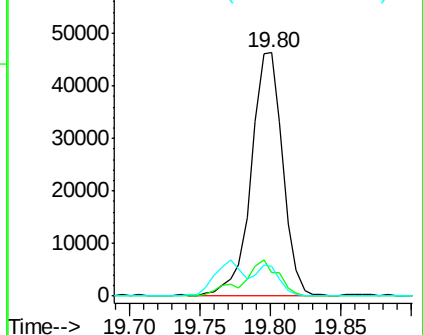

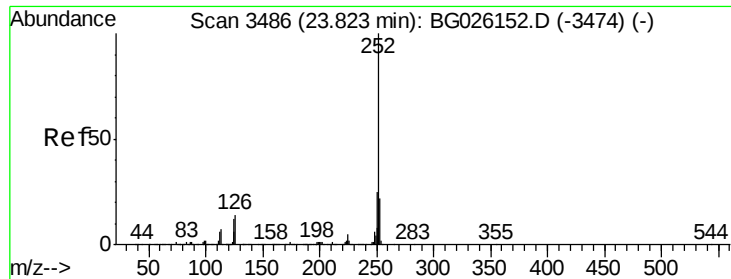

#24

Benzo(b)fluoranthene

Concen: 1.15 ng/ul

RT: 23.83 min Scan# 3487

Delta R.T. 0.00 min

Lab File: BG026161.D


Acq: 9 Mar 2017 22:34

Instrument :

BNA_G

ClientSampleId :

C0AJ5

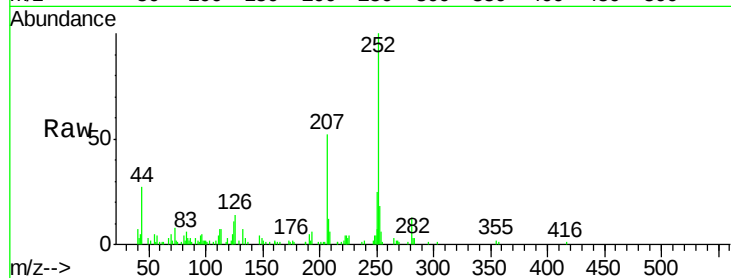

Tgt Ion:252 Resp: 50637

Ion Ratio Lower Upper

252 100

253 18.0 17.8 26.6

125 10.9 9.4 14.0

