
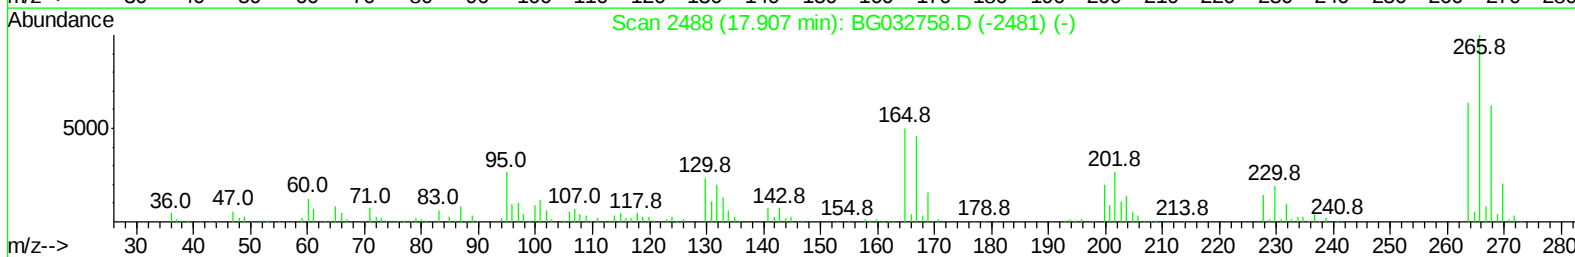
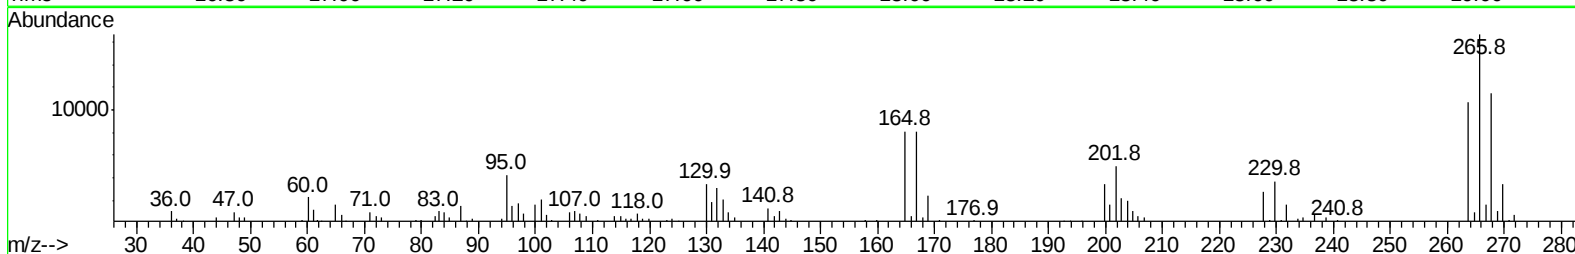


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030918\
Data File : BG033070.D
Acq On : 9 Mar 2018 13:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 04:35:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 15:10:14 2018
Response via : Initial Calibration

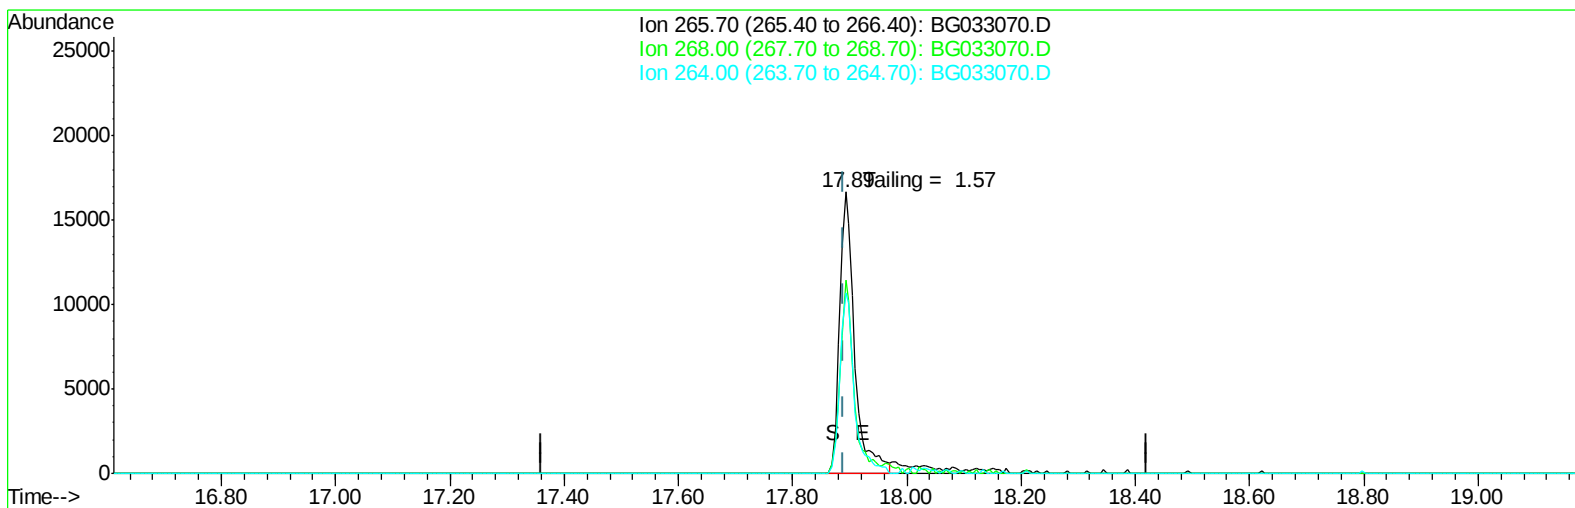

TIC: BG033070.D

(69) Pentachlorophenol (C)




17.892min (+0.001) 79503.13ng

response 30328

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	68.84
264.00	62.00	64.20
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA G\DATA\BG030918\
Data File : BG033070.D
Acq On : 9 Mar 2018 13:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 04:35:05 2018
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG022118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 09 15:10:14 2018
Response via : Initial Calibration

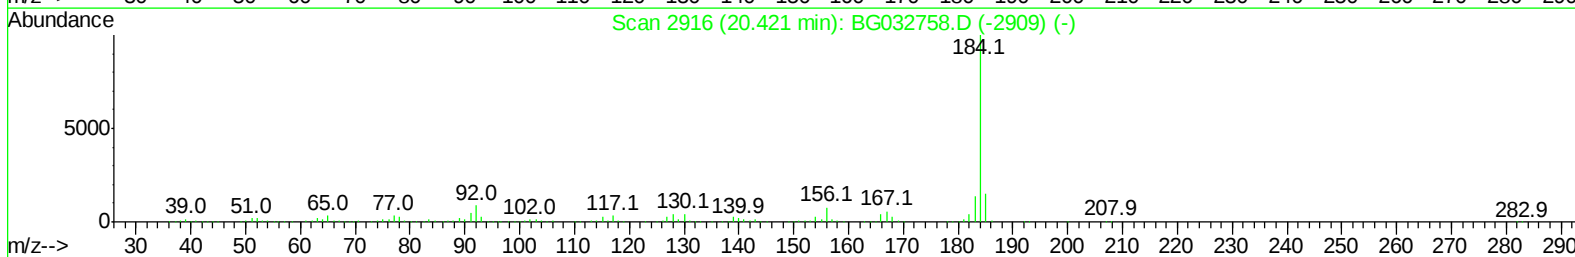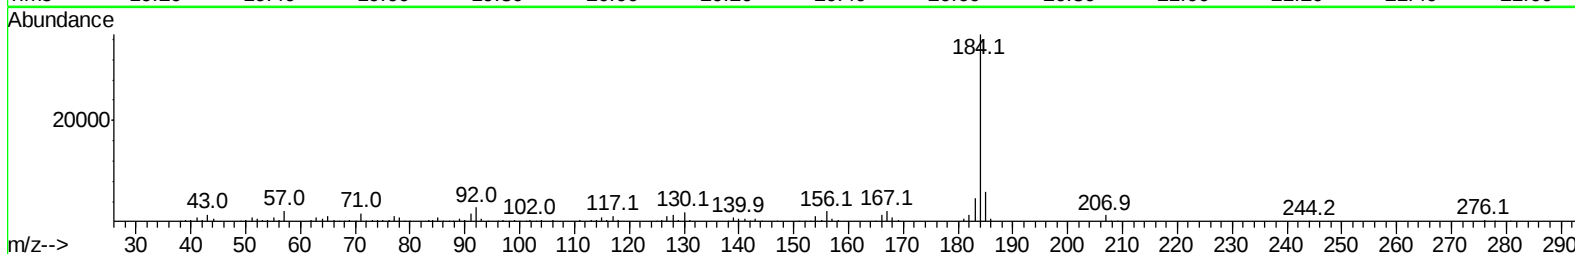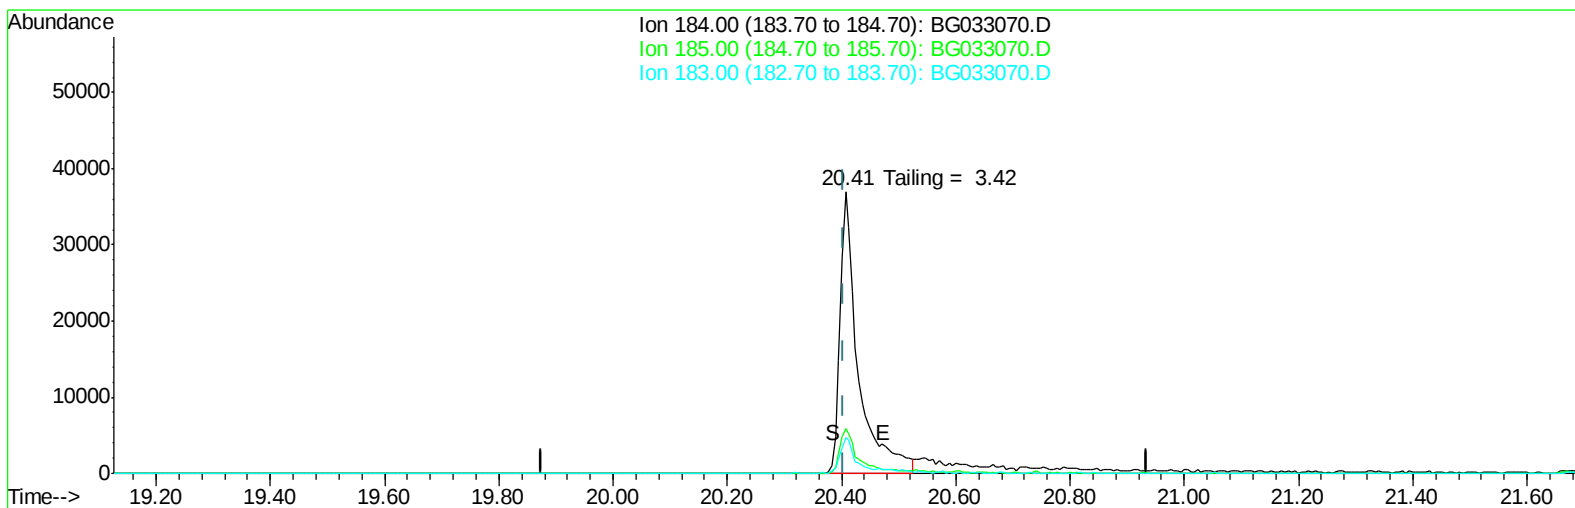

TIC: BG033070.D

(76) Benzidine

20.407min (+0.001) 43788.32ng

response 82093

Ion	Exp%	Act%
184.00	100	100
185.00	13.90	15.82
183.00	13.30	12.71
0.00	0.00	0.00