


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA G\Data\BG030918\
Data File : BG033070.D
Acq On : 9 Mar 2018 13:43
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG022118.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 09 15:10:14 2018

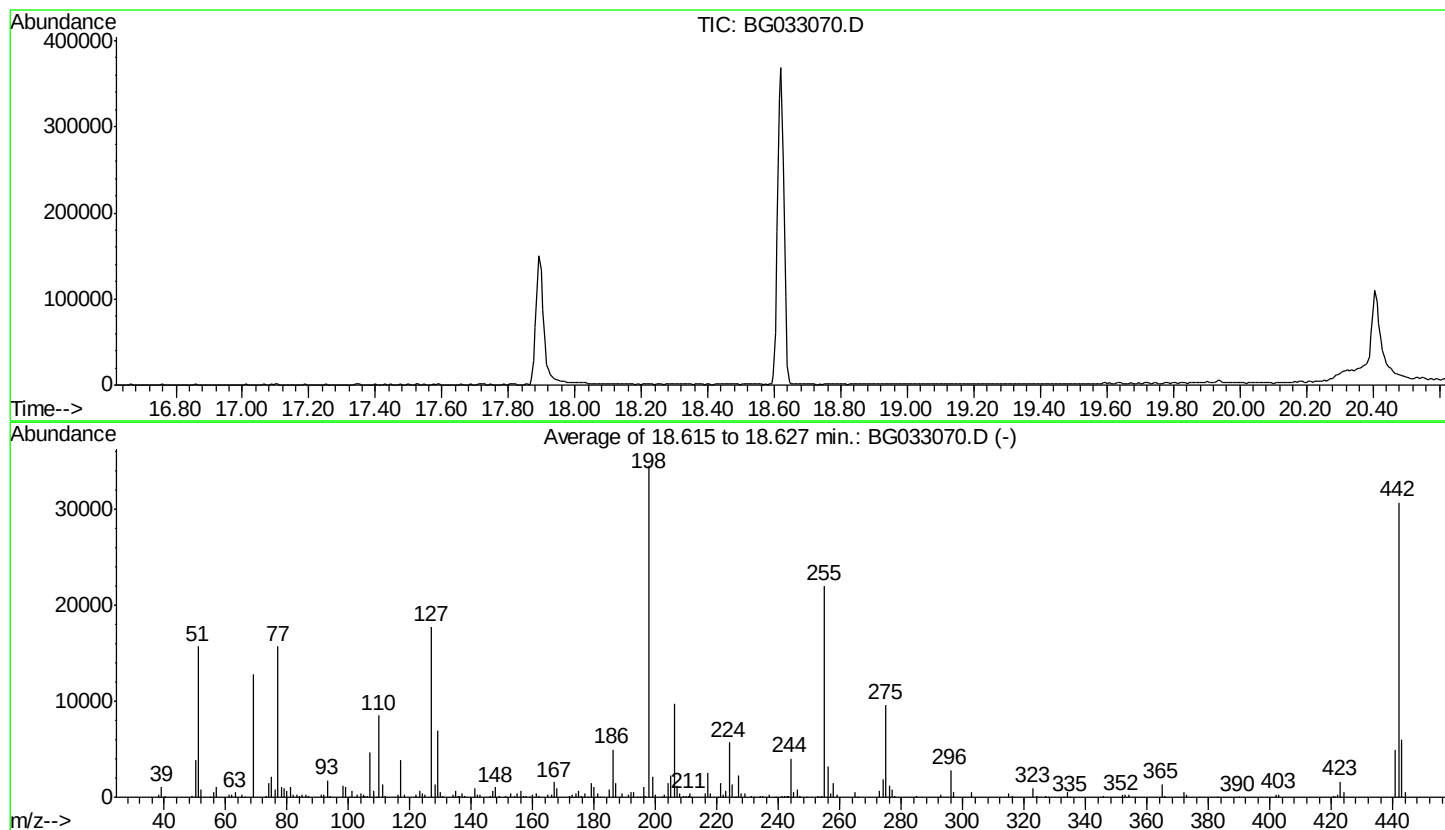

AutoFind: Scans 2609, 2610, 2611; Background Corrected with Scan 2602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.4	15704	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.3	12877	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	17815	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	34568	PASS
199	198	5	9	6.3	2187	PASS
275	198	10	60	27.8	9624	PASS
365	198	1	100	3.9	1352	PASS
441	442	0.01	24	16.0	4908	PASS
442	198	50	100	88.9	30733	PASS
443	442	15	24	19.4	5960	PASS