
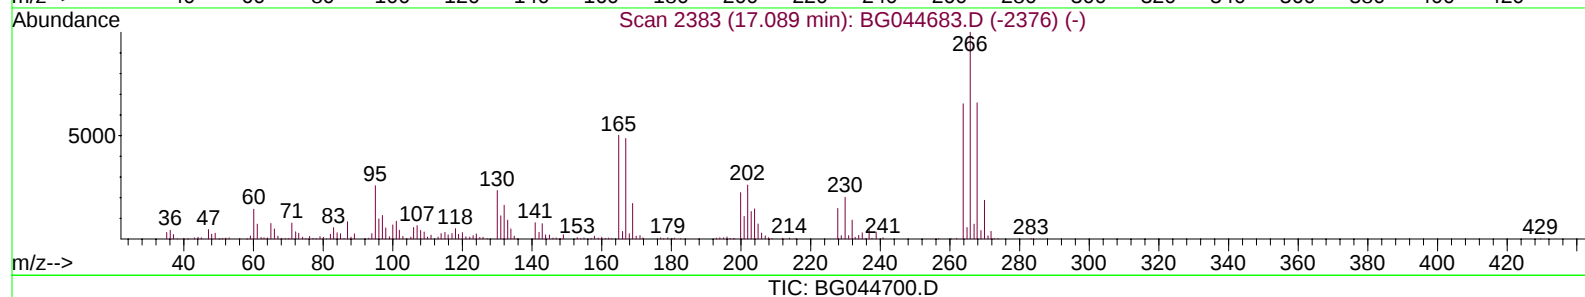
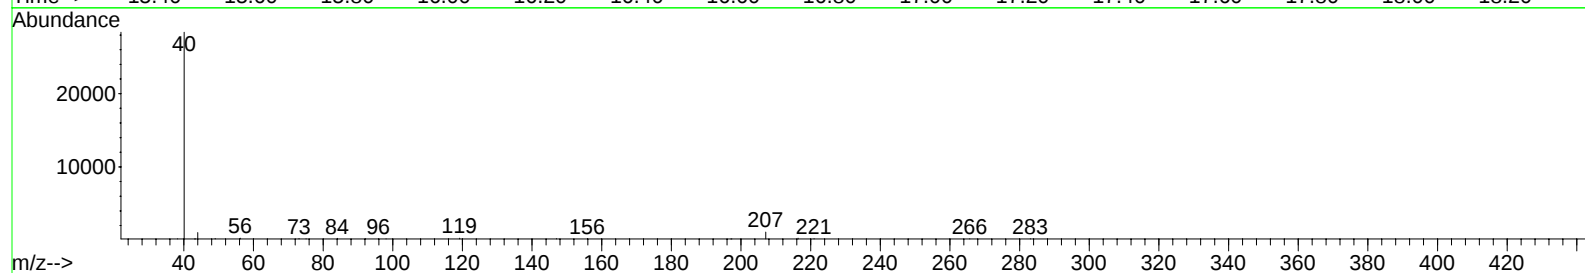


Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG030920\
 Data File : BG044700.D
 Acq On : 9 Mar 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:19:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 17:42:35 2020
 Response via : Initial Calibration

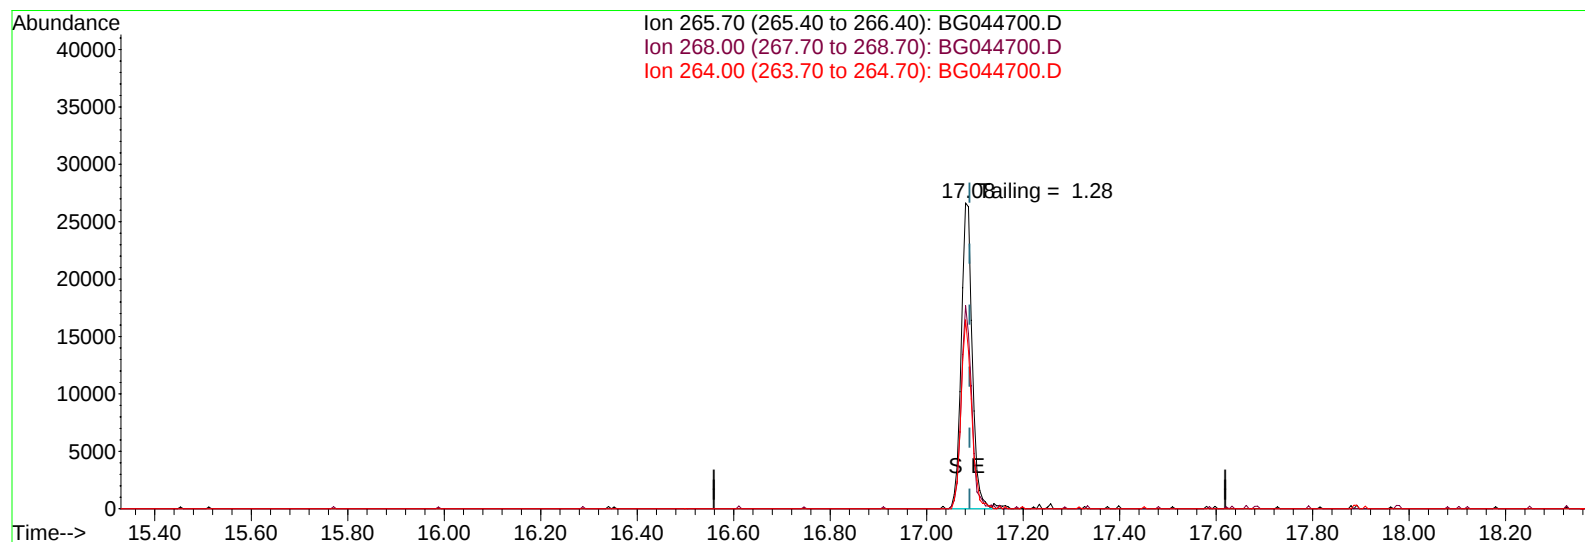

(70) Pentachlorophenol (C)




16.340min (-0.749) 170.27ng

response 125

Ion	Exp%	Act%
265.70	100	100
268.00	65.90	0.00#
264.00	65.40	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA G\Data\BG030920\
 Data File : BG044700.D
 Acq On : 9 Mar 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 19:19:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG030520.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 05 17:42:35 2020
 Response via : Initial Calibration

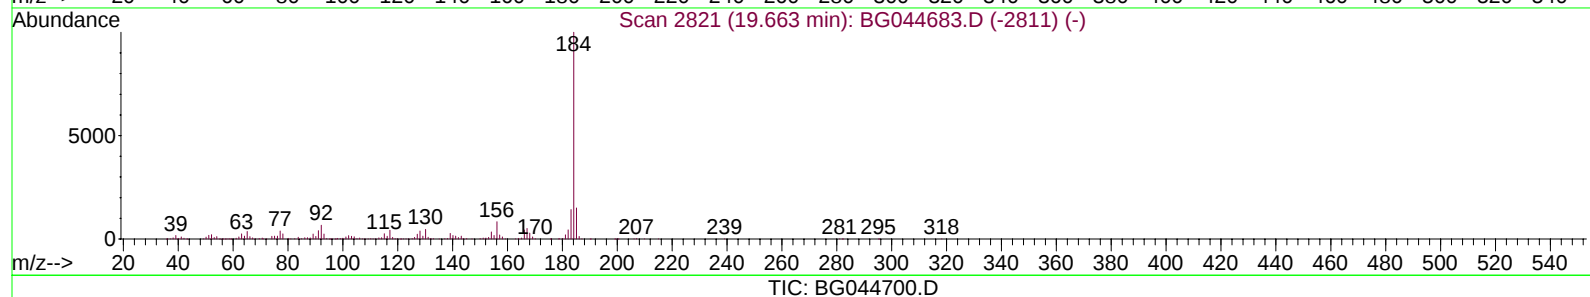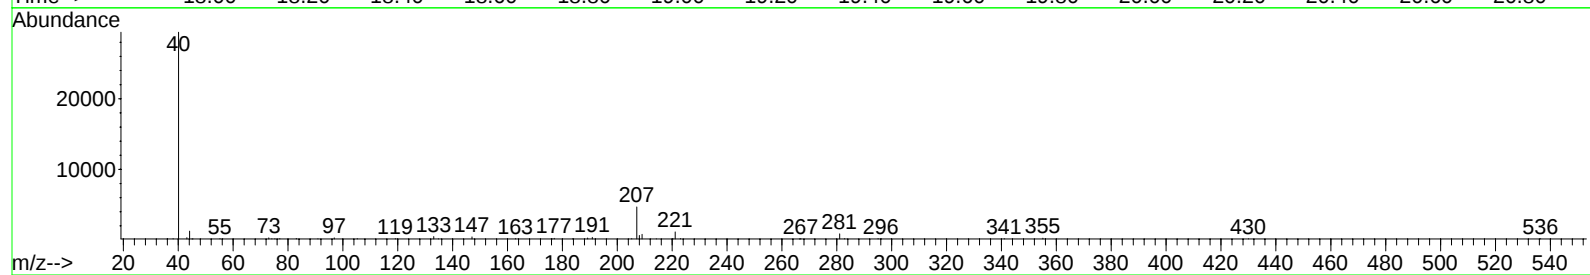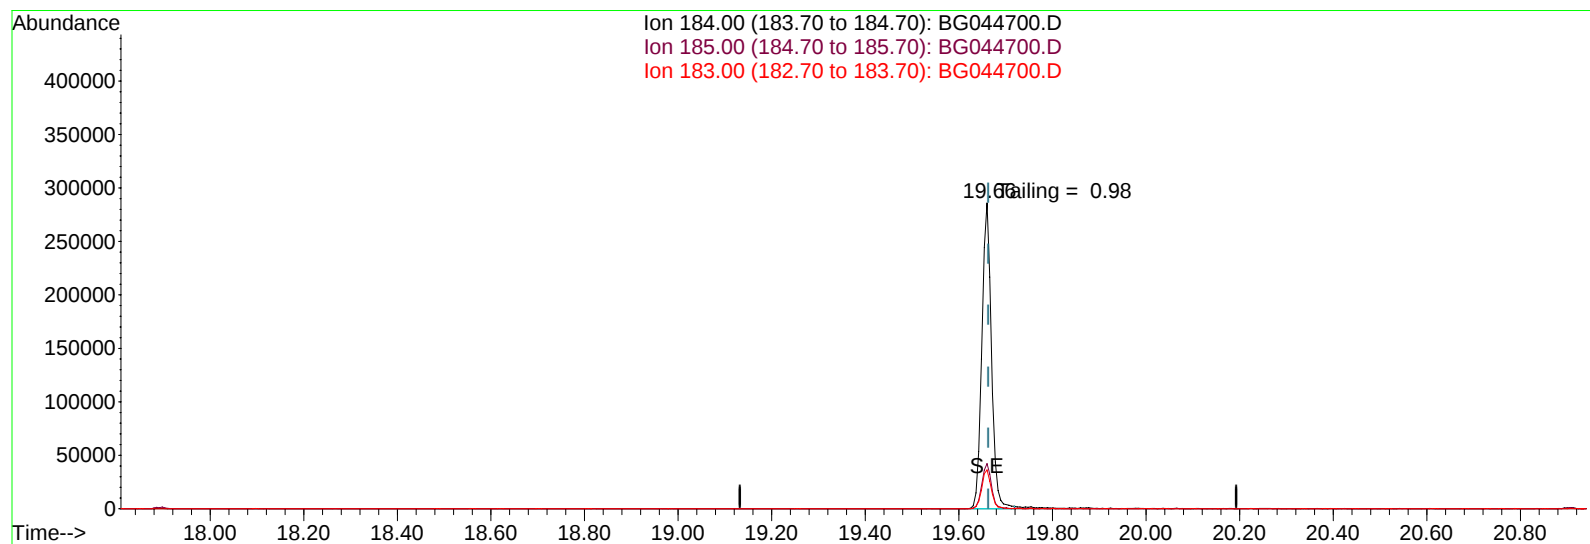

(77) Benzidine

18.820min (-0.843) 0.77ng

response 63

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	0.00#
183.00	14.30	100.00#
0.00	0.00	0.00