


Data Path : Z:\SVOASRV\HPCHEM1\BNA_G\DATA\BG030920\
 Data File : BG044700.D
 Acq On : 9 Mar 2020 9:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG030520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 05 17:42:35 2020

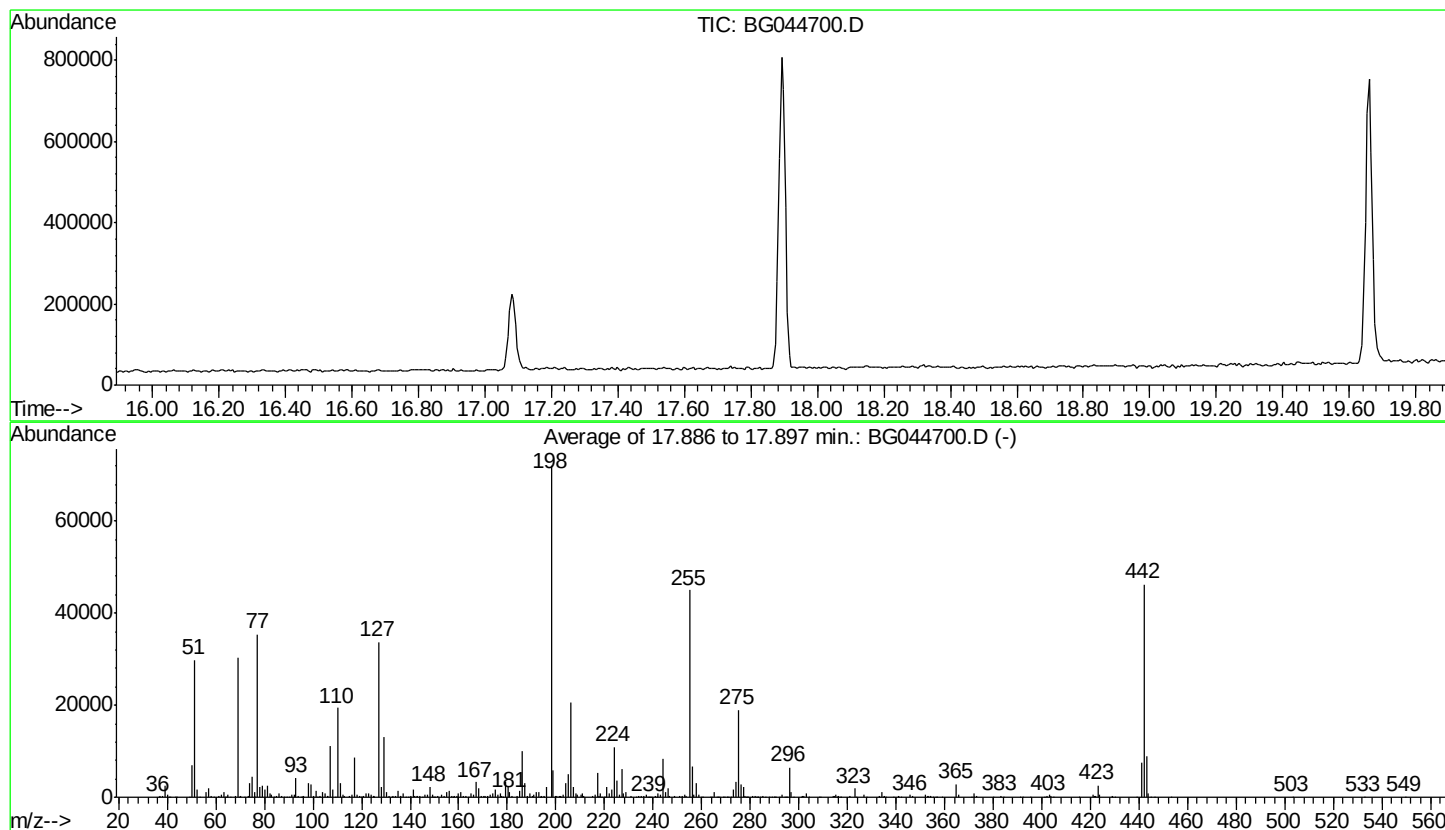

AutoFind: Scans 2518, 2519, 2520; Background Corrected with Scan 2512

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	29854	PASS
68	69	0.00	2	1.2	377	PASS
69	198	0.00	100	41.9	30189	PASS
70	69	0.00	2	1.0	295	PASS
127	198	10	80	46.8	33749	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	72053	PASS
199	198	5	9	8.0	5768	PASS
275	198	10	60	26.3	18969	PASS
365	198	1	100	3.9	2838	PASS
441	198	0.01	100	10.5	7534	PASS
442	198	50	100	64.1	46210	PASS
443	442	15	24	19.2	8867	PASS