
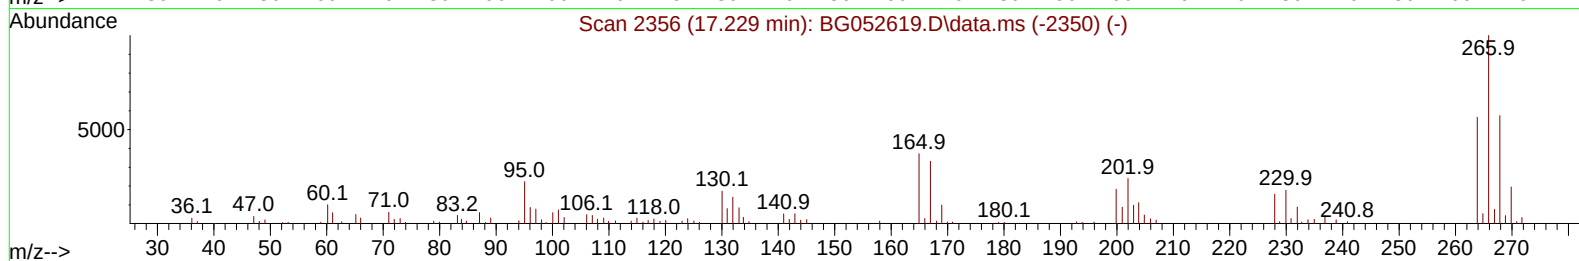
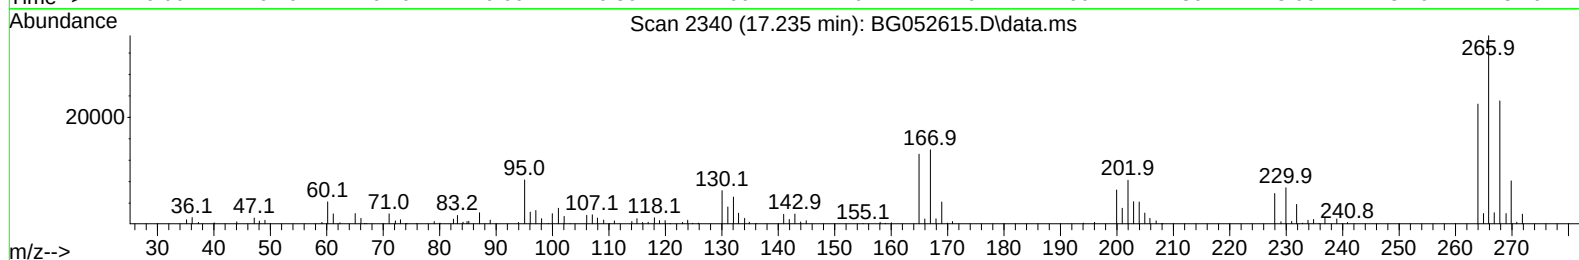


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030922\  
Data File : BG052615.D  
Acq On    : 9 Mar 2022 13:40  
Operator  : CG/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1 Sample Multiplier: 1
```

Quant Time: Mar 10 08:25:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

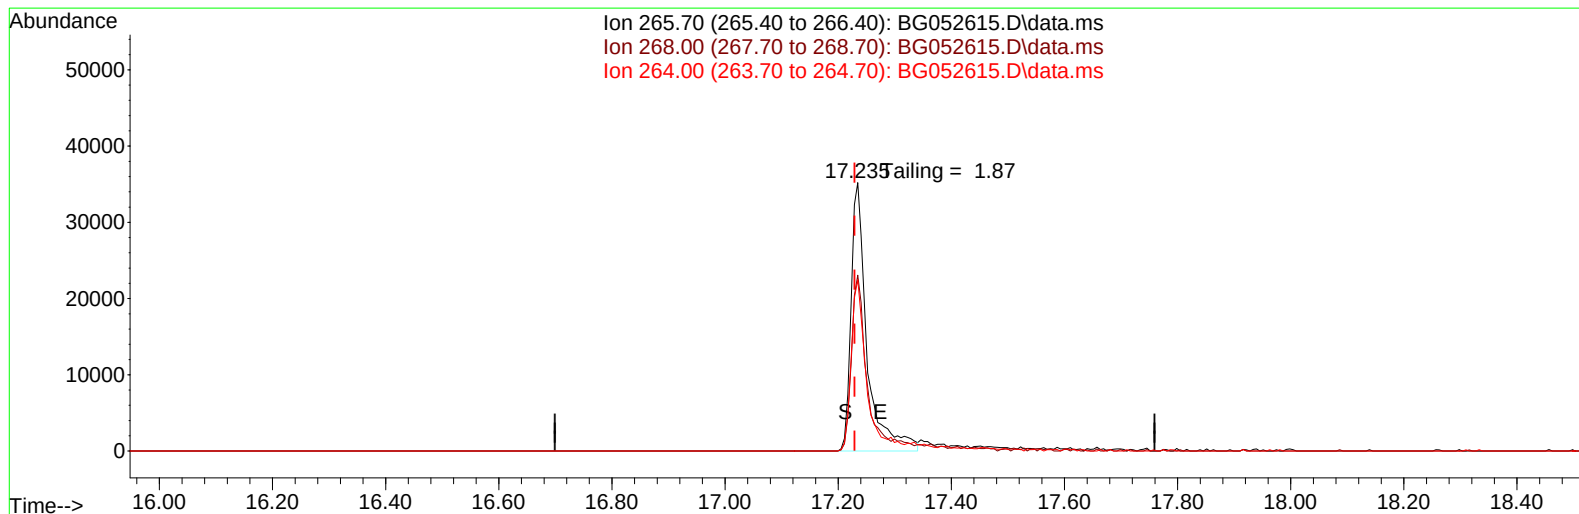

TIC: BG052615.D\data.ms

(70) Pentachlorophenol (C)




17.235min (+ 0.006) 70064.83 ng

response 69363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.51
264.00	56.60	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030922\
Data File : BG052615.D
Acq On : 9 Mar 2022 13:40
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 10 08:25:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 10 06:37:54 2022
Response via : Initial Calibration

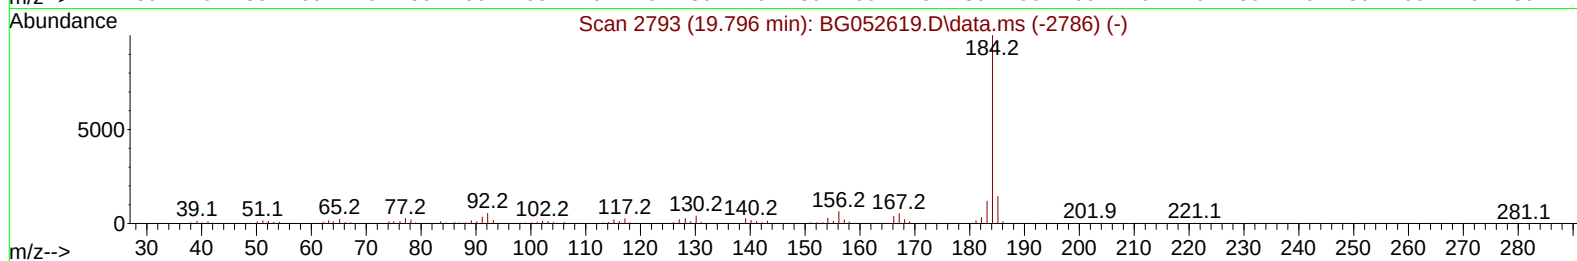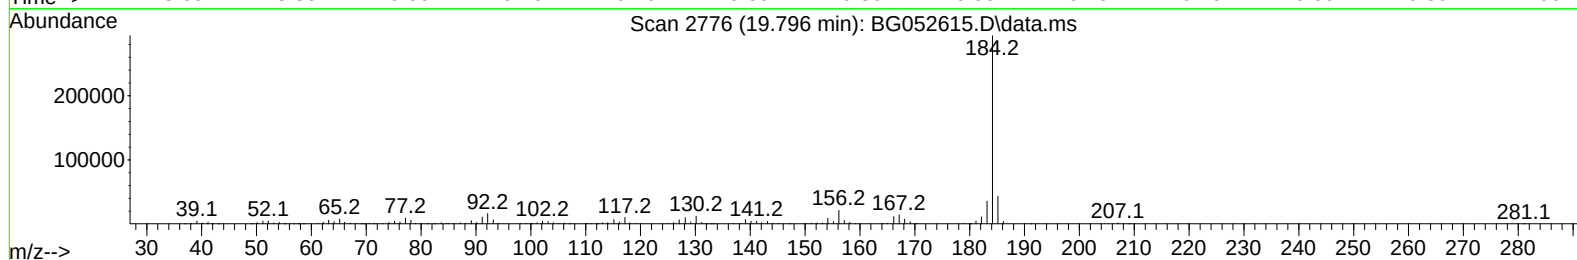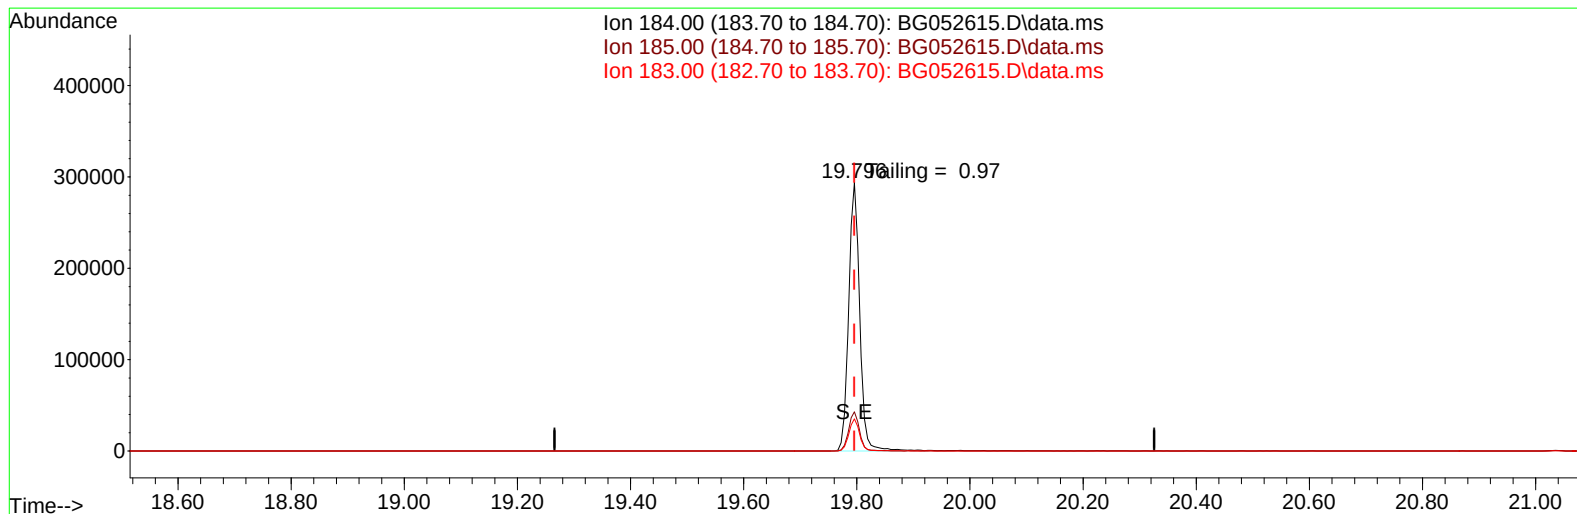

TIC: BG052615.D\data.ms

(77) Benzidine**19.796min (+ 0.000) 331216.45 ng****response 398514**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.63
183.00	11.80	12.02
0.00	0.00	0.00