
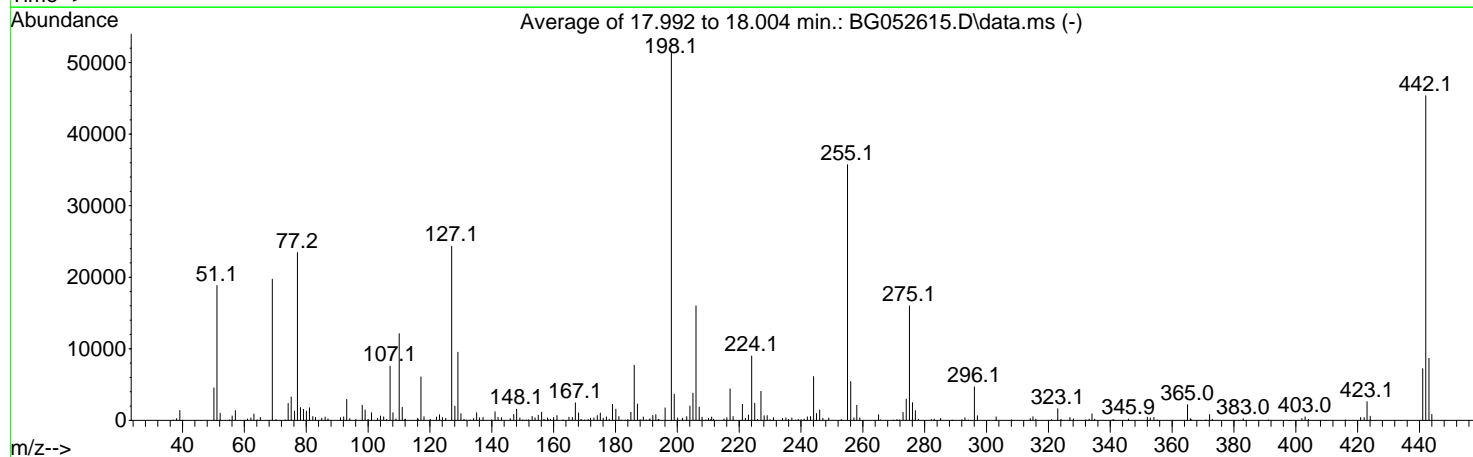


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030922\
 Data File : BG052615.D
 Acq On : 9 Mar 2022 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 10 06:37:54 2022

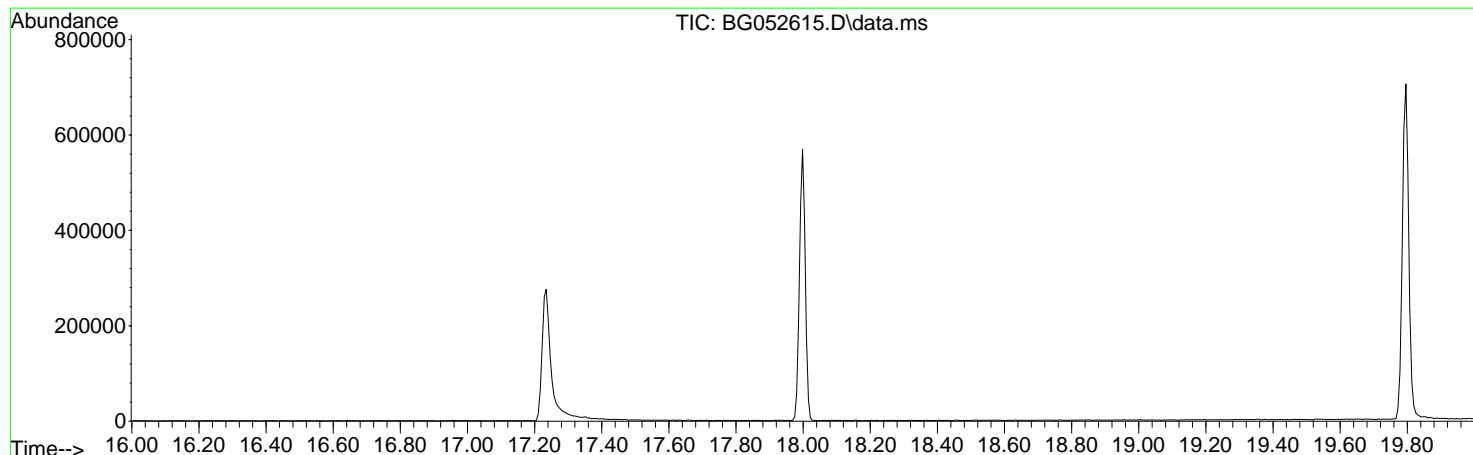

AutoFind: Scans 2469, 2470, 2471; Background Corrected with Scan 2462

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.6	18841	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.4	19718	PASS
70	69	0.00	2	0.6	115	PASS
127	198	10	80	47.3	24323	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	51408	PASS
199	198	5	9	7.1	3660	PASS
275	198	10	60	31.1	15981	PASS
365	198	1	100	4.3	2199	PASS
441	198	0.01	100	14.1	7235	PASS
442	442	50	100	100.0	45365	PASS
443	442	15	24	19.1	8686	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/9/2022	BNA_G	<u>BG052615.D</u>
Compound Name	Response	Retention Time
DDT	206577	21.035
DDD	2577	20.589
DDE	176	20.084
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2753	209330	1.32

Instrument :
 BNA_G
 ClientSampled :
 DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030922\
 Data File : BG052615.D
 Acq On : 9 Mar 2022 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
ClientSampleId :
 DFTPP

Quant Time: Mar 10 08:25:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 06:37:54 2022
 Response via : Initial Calibration

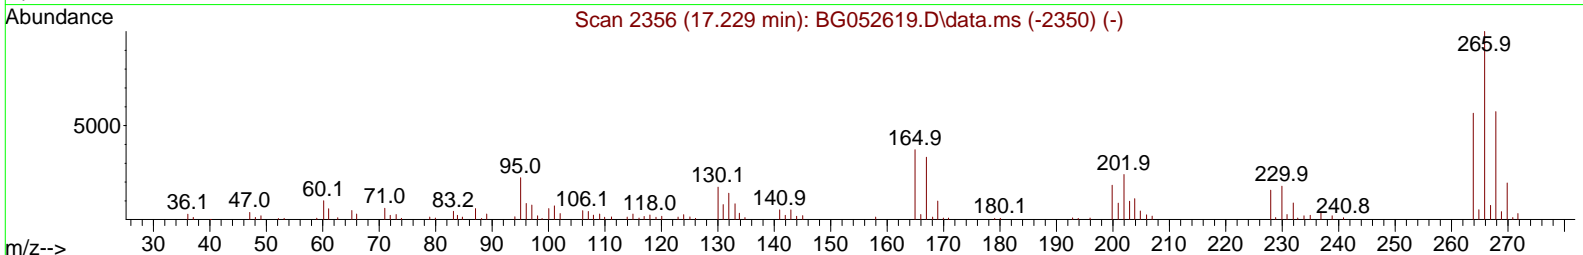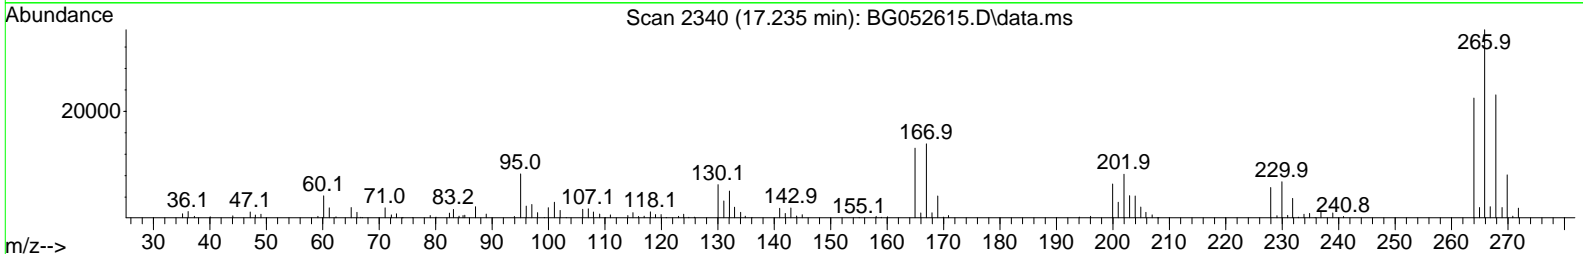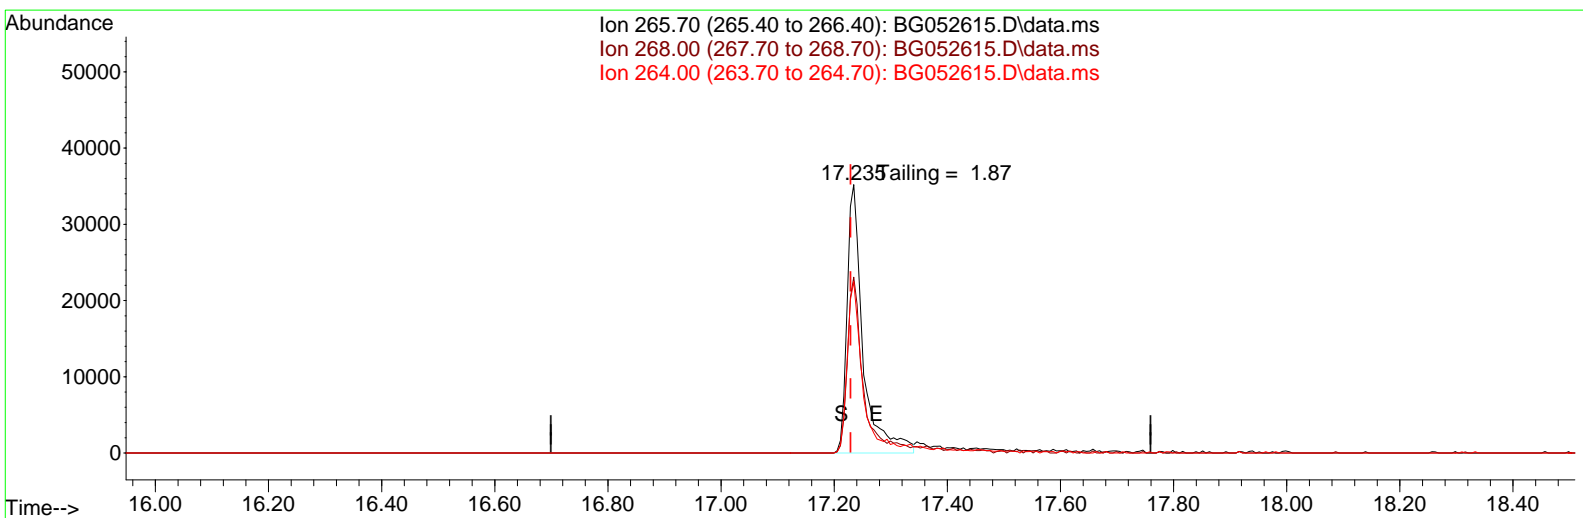

TIC: BG052615.D\data.ms

(70) Pentachlorophenol (C)

17.235min (+ 0.006) 70064.83 ng




response 69363

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	57.40	65.51
264.00	56.60	63.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG030922\
 Data File : BG052615.D
 Acq On : 9 Mar 2022 13:40
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Mar 10 08:25:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG030922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 10 06:37:54 2022
 Response via : Initial Calibration

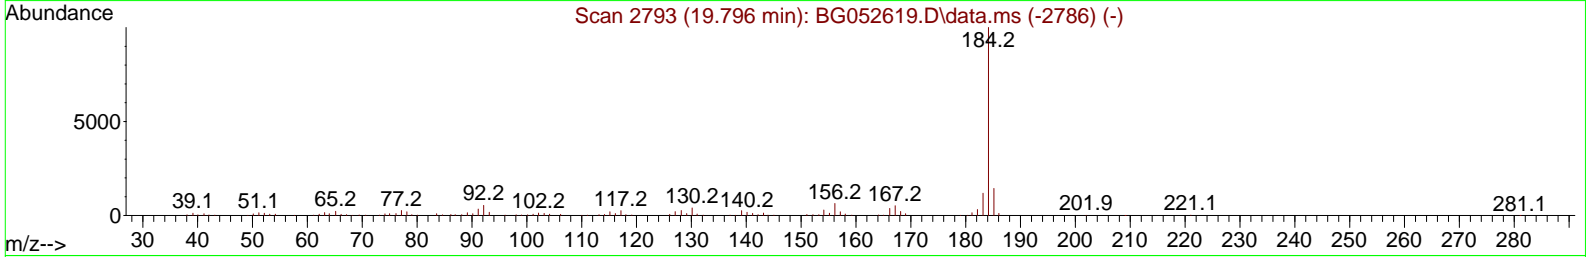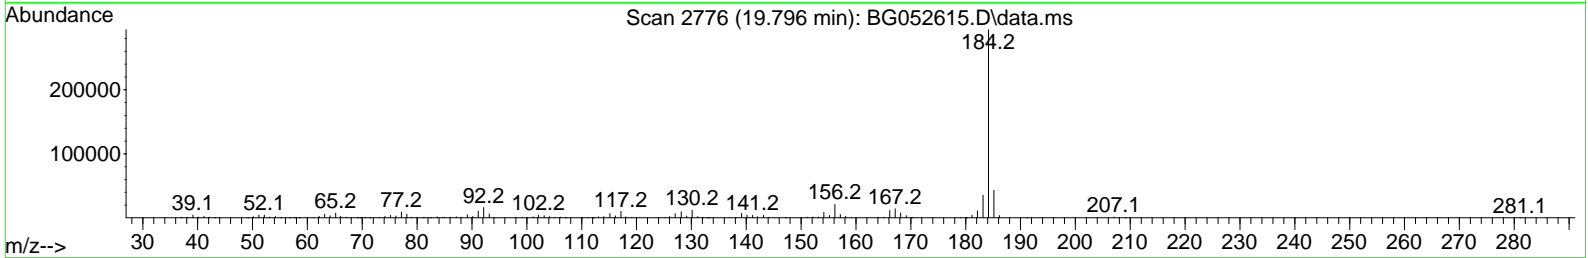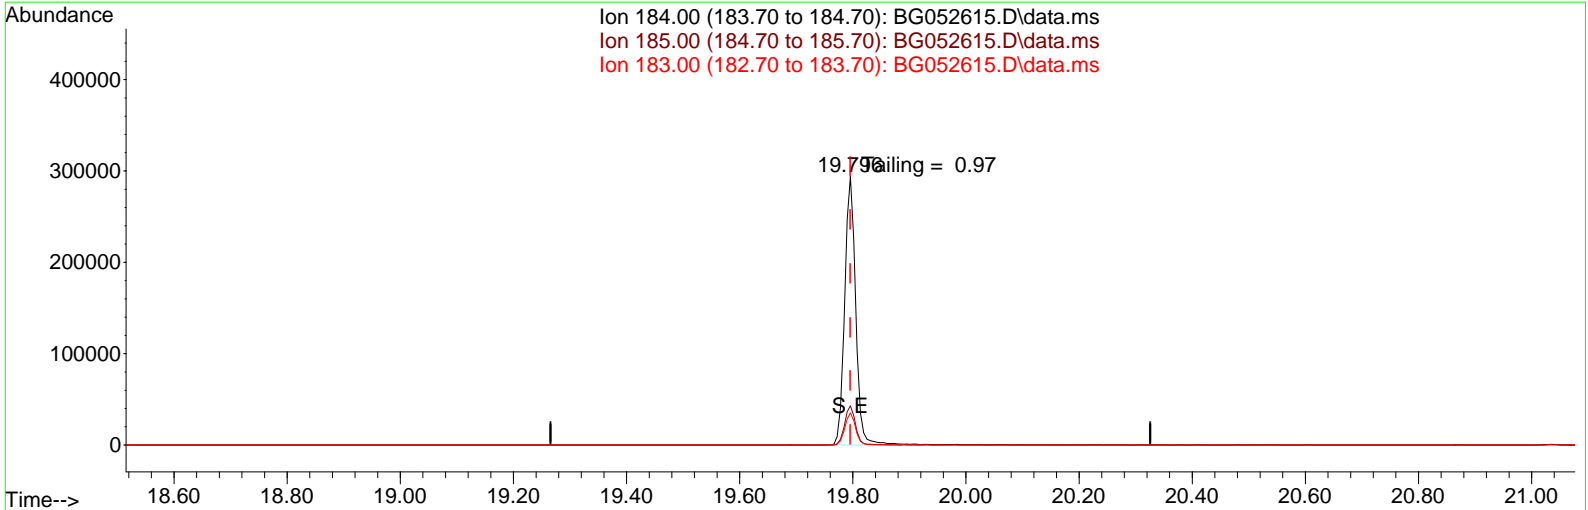

TIC: BG052615.D\data.ms

(77) Benzidine

19.796min (+ 0.000) 331216.45 ng

response 398514

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.63
183.00	11.80	12.02
0.00	0.00	0.00