


Data Path : S:\HPCHEM1\BNA_G\DATA\BG031016\
Data File : BG021394.D
Acq On : 10 Mar 2016 3:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP06

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG031016.M
Title : SVOA CALIBRATION
Last Update : Fri Mar 11 00:30:31 2016

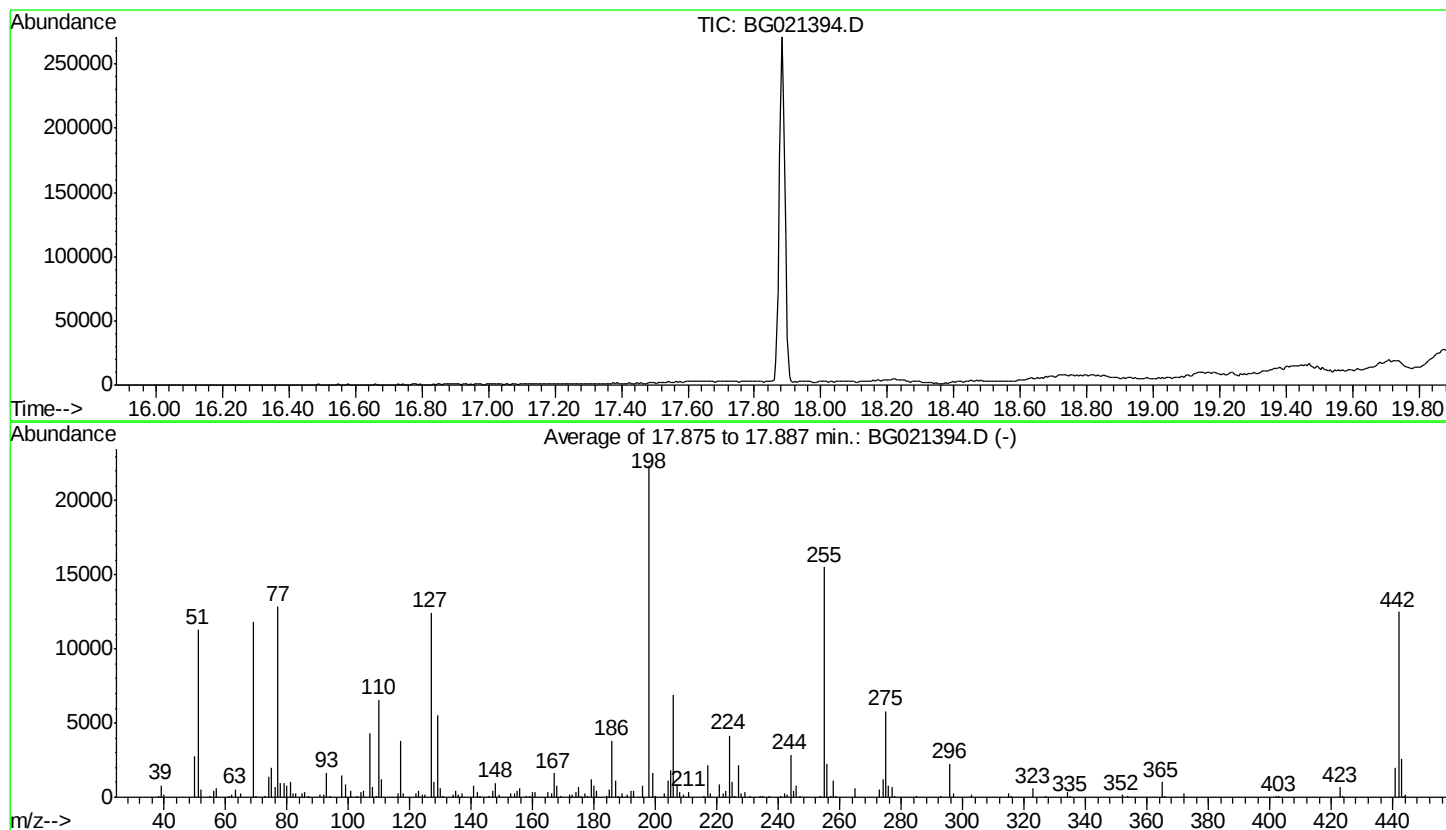

AutoFind: Scans 2559, 2560, 2561; Background Corrected with Scan 2554

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	11290	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	52.9	11825	PASS
70	69	0.00	2	0.5	54	PASS
127	198	10	80	55.6	12436	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	22368	PASS
199	198	5	9	7.5	1684	PASS
275	198	10	60	25.9	5800	PASS
365	198	1	100	4.6	1024	PASS
441	442	0.01	100	15.7	1970	PASS
442	198	50	100	55.9	12512	PASS
443	442	15	24	20.8	2607	PASS

m/z	Abundance
41.00	152.0
43.00	491.0
43.90	159.0
55.00	241.0
57.00	449.0
69.00	213.0
71.00	247.0
140.90	396.0
155.00	247.0
167.00	217.0
169.00	156.0
206.80	169.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

m/z	Abundance
39.00	760.0
39.90	186.0
40.90	211.0
43.00	477.0
50.00	2511.0
51.00	10242.0
52.00	556.0
55.00	266.0
55.90	333.0
56.90	885.0
61.00	194.0
62.00	204.0
63.00	577.0
65.00	255.0
68.90	11349.0
71.00	214.0
72.90	211.0
74.00	1352.0
74.90	1632.0
76.00	479.0
77.00	11559.0
78.00	970.0
78.90	878.0
79.90	782.0
80.90	855.0
81.90	178.0
83.00	292.0
84.90	241.0
85.90	297.0
91.90	186.0
92.90	1460.0
97.90	1196.0
98.90	723.0
100.90	369.0
103.90	206.0
104.90	352.0
106.90	3800.0
107.90	523.0
108.90	177.0
109.90	5543.0
110.90	1131.0
115.90	215.0
116.90	3029.0
117.90	203.0
122.00	262.0
122.90	426.0
123.80	150.0
124.90	202.0
126.90	9821.0
127.90	932.0
128.90	4437.0
129.90	498.0
133.90	209.0
134.90	384.0
135.90	154.0
136.90	220.0
140.90	1135.0
141.90	313.0
146.90	310.0
147.90	803.0
148.90	187.0
152.90	253.0
153.90	312.0
154.90	648.0
155.90	506.0
159.90	244.0
160.90	279.0
164.80	280.0
165.90	211.0
166.90	1493.0
167.90	626.0
168.90	235.0
173.80	258.0
174.90	565.0
176.90	207.0
177.80	154.0
178.90	970.0
179.90	433.0
180.80	299.0
184.90	430.0
185.90	3028.0
186.90	773.0
188.90	247.0
191.90	317.0
192.90	361.0
195.80	708.0
197.80	17808.0
198.80	1458.0
202.90	163.0
203.90	830.0
204.90	1419.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

205.90	5147.0
206.90	736.0
207.90	345.0
208.90	164.0
210.90	283.0
216.80	1830.0
217.80	198.0
220.80	795.0
221.70	197.0
222.80	324.0
223.90	3320.0
224.90	792.0
226.80	1499.0
227.90	275.0
228.90	312.0
241.90	165.0
243.90	2191.0
244.90	360.0
245.90	543.0
254.90	11851.0
255.80	1543.0
257.80	716.0
264.90	455.0
272.80	317.0
273.90	1035.0
274.90	4089.0
275.90	631.0
276.90	464.0
295.80	1596.0
296.90	239.0
314.80	183.0
322.80	428.0
333.90	205.0
364.80	583.0
371.80	190.0
422.90	380.0
440.90	1004.0
441.90	7030.0
442.80	1499.0
443.70	207.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

m/z	Abundance
38.00	158.0
39.00	990.0
39.90	171.0
43.00	486.0
43.90	167.0
50.00	3357.0
51.00	13602.0
52.00	670.0
55.00	325.0
56.00	430.0
57.00	1348.0
60.90	190.0
62.10	187.0
63.00	704.0
64.90	274.0
68.90	14264.0
70.00	163.0
71.00	246.0
74.00	1563.0
75.00	2345.0
76.00	837.0
77.00	15301.0
78.00	942.0
78.90	980.0
79.90	924.0
80.90	1249.0
81.90	369.0
82.90	301.0
84.90	331.0
85.90	503.0
87.00	161.0
90.90	319.0
91.90	345.0
92.90	1958.0
93.90	179.0
97.90	1951.0
98.90	1055.0
100.90	555.0
103.90	453.0
104.90	429.0
106.90	5223.0
107.90	895.0
109.90	7984.0
110.90	1349.0
115.90	235.0
116.90	4400.0
117.90	344.0
121.90	376.0
122.90	683.0
124.90	208.0
126.90	15006.0
127.90	1266.0
128.90	6503.0
129.90	690.0
133.90	178.0
134.90	563.0
135.80	158.0
136.90	249.0
140.90	1264.0
142.00	308.0
142.90	211.0
145.80	167.0
146.90	560.0
147.90	1208.0
149.00	255.0
152.90	291.0
154.00	270.0
154.90	723.0
155.90	794.0
157.80	204.0
158.90	175.0
159.90	334.0
160.90	487.0
164.90	421.0
166.00	368.0
166.90	2239.0
167.90	853.0
168.90	267.0
171.80	247.0
172.80	219.0
173.90	376.0
174.90	684.0
175.90	205.0
176.90	385.0
178.90	1470.0
179.90	1022.0
180.90	548.0
183.90	166.0
184.90	723.0
185.90	4497.0
186.90	1216.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

187.80	173.0
188.80	397.0
190.80	186.0
191.90	482.0
192.90	580.0
195.80	866.0
197.80	26712.0
198.90	2112.0
199.80	228.0
202.90	335.0
203.90	1293.0
204.90	2054.0
205.90	8538.0
206.90	1150.0
207.90	378.0
208.70	236.0
210.90	429.0
215.90	190.0
216.80	2455.0
217.90	296.0
220.80	888.0
221.80	292.0
222.90	524.0
223.90	5183.0
224.90	1389.0
226.90	2609.0
227.90	291.0
228.80	399.0
233.80	174.0
234.80	168.0
236.90	216.0
240.80	196.0
241.90	233.0
242.90	285.0
243.90	3539.0
244.90	555.0
245.80	1026.0
246.80	186.0
253.80	185.0
254.90	18248.0
255.90	2711.0
256.80	179.0
257.90	1620.0
258.80	163.0
264.90	664.0
272.90	624.0
273.90	1328.0
274.90	7153.0
275.90	1000.0
276.90	840.0
277.90	195.0
284.90	156.0
295.90	2830.0
296.90	306.0
302.90	252.0
314.90	335.0
315.90	170.0
322.90	663.0
326.80	170.0
333.80	396.0
351.80	216.0
353.80	169.0
364.90	1275.0
365.90	195.0
371.90	329.0
422.90	875.0
423.90	215.0
440.90	2335.0
441.90	14473.0
442.90	3092.0
443.90	262.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

m/z	Abundance
39.00	591.0
40.00	157.0
41.00	209.0
43.00	391.0
50.00	2490.0
51.00	10028.0
52.00	459.0
55.00	289.0
55.90	488.0
57.00	1030.0
62.00	192.0
63.00	408.0
65.00	176.0
68.90	10503.0
71.00	194.0
74.00	1354.0
74.90	1898.0
76.00	716.0
77.00	11729.0
77.90	868.0
78.90	935.0
79.90	540.0
80.90	991.0
81.90	245.0
82.90	277.0
85.00	193.0
85.90	236.0
90.90	217.0
92.90	1580.0
97.90	1258.0
98.90	808.0
100.90	471.0
102.80	207.0
103.90	327.0
104.90	413.0
106.90	3861.0
107.90	610.0
109.00	168.0
109.90	6224.0
110.90	1070.0
116.00	267.0
116.90	3860.0
117.90	272.0
121.80	222.0
122.90	321.0
123.90	295.0
126.90	12482.0
127.90	956.0
128.90	5533.0
129.90	531.0
130.90	186.0
133.90	184.0
134.80	352.0
135.90	218.0
136.90	191.0
140.90	1116.0
141.90	312.0
146.80	402.0
147.90	937.0
148.90	201.0
153.00	255.0
153.90	232.0
154.90	643.0
155.90	517.0
159.90	387.0
160.90	304.0
164.90	322.0
166.00	332.0
166.90	1787.0
167.90	770.0
168.90	313.0
171.80	158.0
172.80	188.0
173.90	368.0
174.90	735.0
176.90	251.0
178.90	1128.0
179.90	907.0
180.90	428.0
184.90	519.0
185.90	3889.0
186.90	1357.0
188.80	238.0
190.90	237.0
191.80	434.0
192.90	412.0
195.90	851.0
197.80	22584.0
198.80	1482.0
202.90	241.0
203.90	1156.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06

204.90	2094.0
205.90	7026.0
206.90	1282.0
207.80	208.0
208.90	178.0
210.90	339.0
215.80	154.0
216.80	2323.0
217.80	298.0
220.80	867.0
221.80	249.0
222.80	540.0
223.90	4015.0
224.80	1004.0
225.90	206.0
226.90	2270.0
227.80	222.0
228.80	342.0
230.90	168.0
233.90	198.0
234.80	153.0
236.90	152.0
242.00	318.0
242.90	265.0
243.90	2954.0
244.90	379.0
245.90	874.0
254.90	16504.0
255.90	2473.0
256.80	183.0
257.80	1097.0
258.80	159.0
264.90	578.0
272.80	615.0
273.90	1157.0
274.90	6158.0
275.90	733.0
276.90	775.0
284.90	175.0
292.90	192.0
295.90	2378.0
296.80	310.0
302.90	290.0
314.90	260.0
315.90	221.0
322.90	657.0
326.80	172.0
333.90	409.0
334.90	180.0
351.80	212.0
353.70	165.0
364.80	1215.0
365.90	198.0
371.90	274.0
401.80	161.0
402.90	180.0
422.90	771.0
423.70	178.0
440.90	2571.0
441.90	16035.0
442.90	3232.0
443.90	250.0

Instrument :
BNA_G
ClientSampleId :
DFTPP06