

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
 Data File : BG026189.D
 Acq On : 11 Mar 2017 1:19
 Operator : SJ/MA
 Sample : I2180-20
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C0BF0

Quant Time: Mar 11 02:50:05 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 11 00:32:15 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.06	152	86370	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	387732	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.66	164	231051	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.40	188	571061	20.00	ng/ul	0.00
77) Chrysene-d12	21.64	240	600015	20.00	ng/ul	0.00
85) Perylene-d12	24.83	264	572040	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	6636	3.30	ng/uL	0.00
5) Phenol-d5	7.21	99	43093	6.71	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.38	67	143866	35.49	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	137748	26.56	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	77342	15.41	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	98283	35.09	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	73601	31.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	163956	31.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	7480	1.07	ng/ul	0.00
43) Dimethylphthalate-d6	14.07	166	610314	40.61	ng/ul	0.00
46) Acenaphthylene-d8	14.36	160	864248	42.84	ng/ul	0.00
51) 4-Nitrophenol-d4	14.84	143	10997	3.72	ng/ul	0.00
57) Fluorene-d10	15.65	176	644623	43.50	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.76	200	58231	21.73	ng/ul	0.00
70) Anthracene-d10	17.50	188	1027240	39.64	ng/ul	0.00
78) Pyrene-d10	19.77	212	1153821	46.75	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.61	264	1011347	40.11	ng/ul	0.00


Target Compounds					Ovalue
42) 2-Nitroaniline	13.67	65	2986	1.04 ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
Data File : BG026189.D
Acq On : 11 Mar 2017 1:19
Operator : SJ/MA
Sample : I2180-20
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
C0BF0

Quant Time: Mar 11 02:50:05 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 11 00:32:15 2017
Response via : Initial Calibration

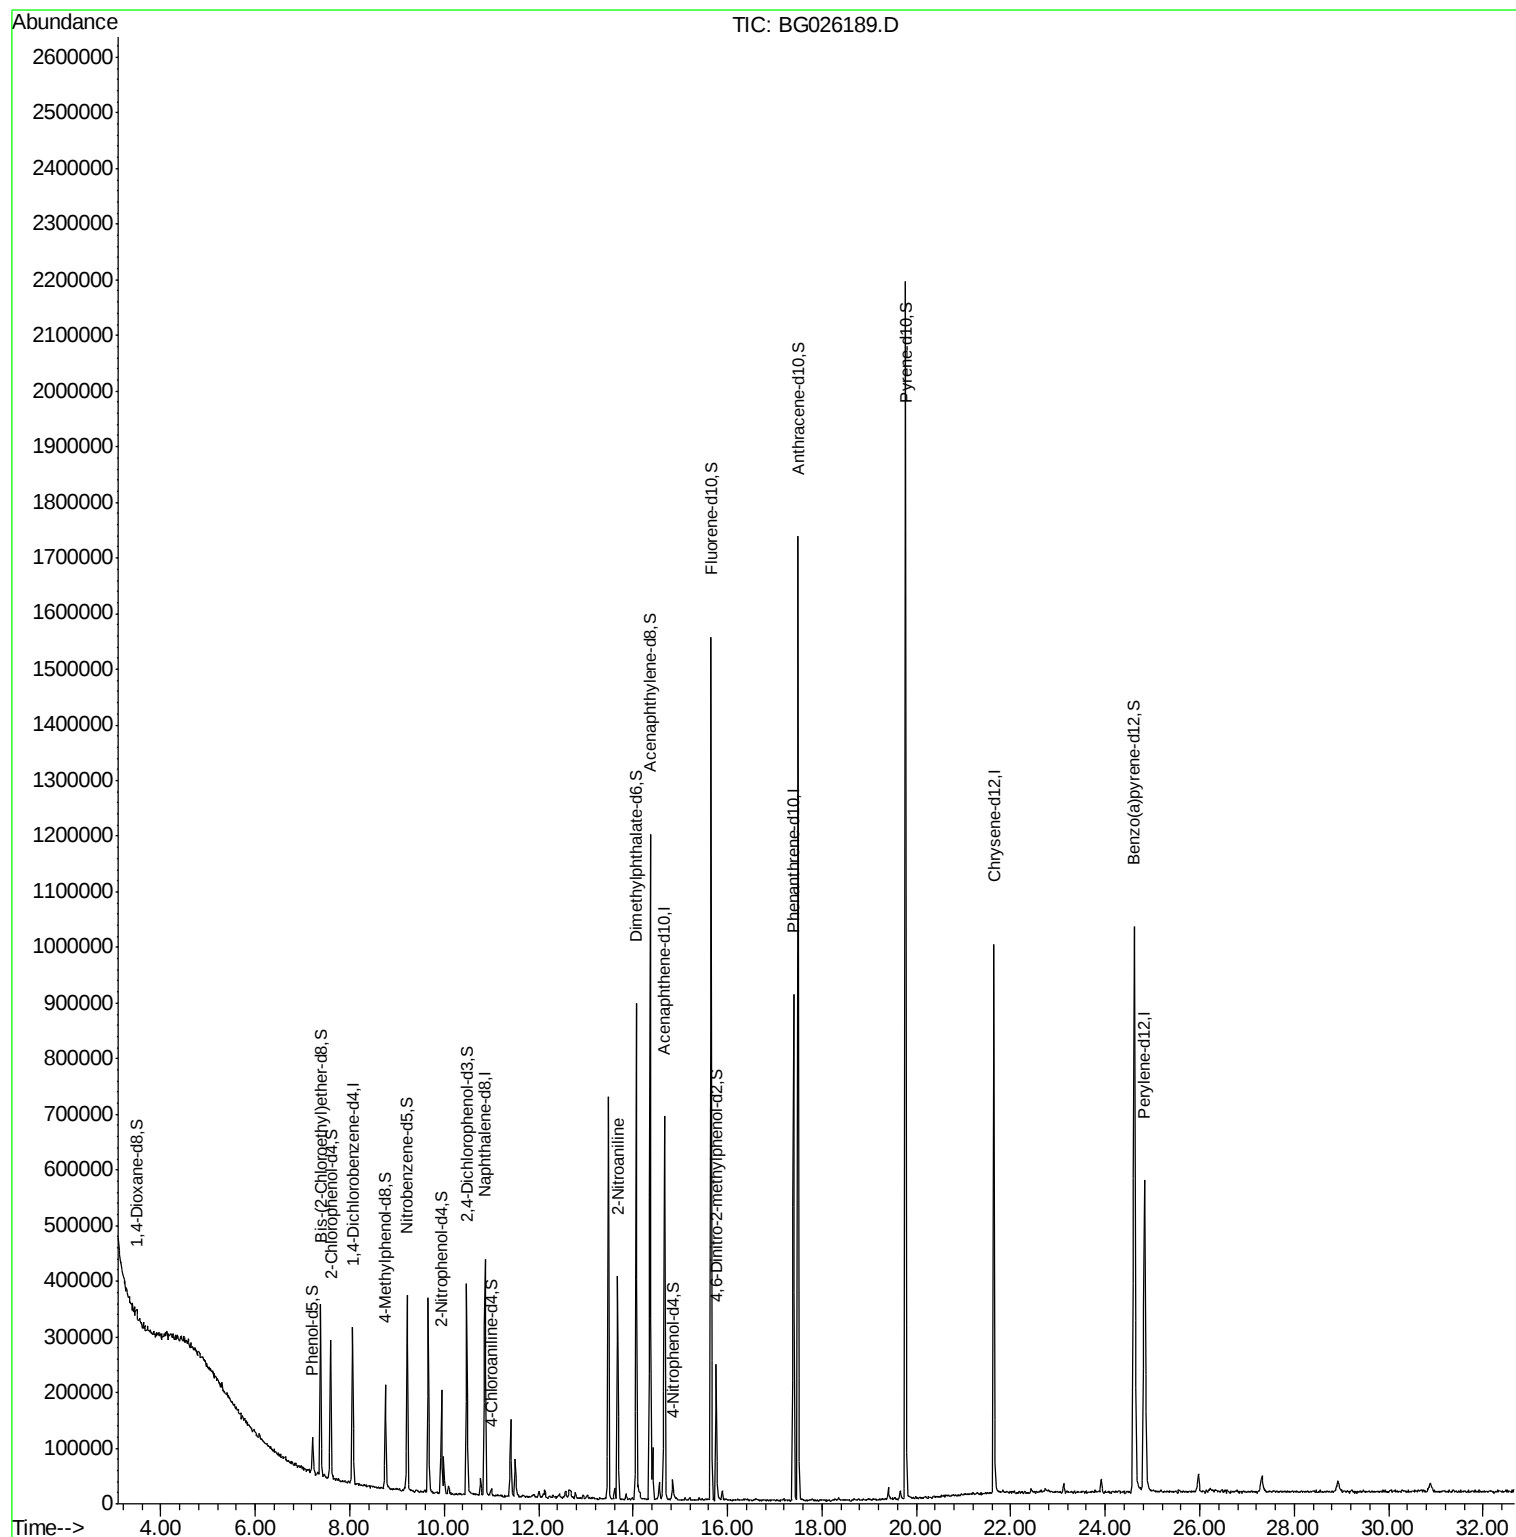

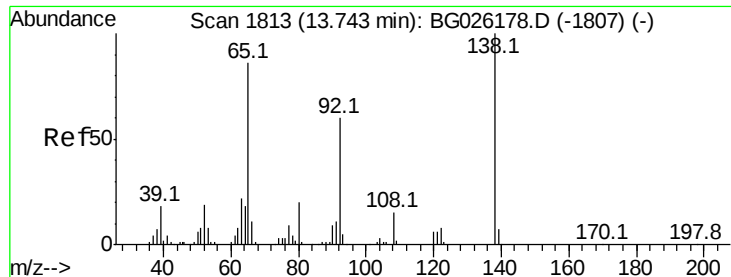

#42
 2-Nitroaniline
 Concen: 1.04 ng/ul
 RT: 13.67 min Scan# 1801
 Delta R.T. -0.07 min
 Lab File: BG026189.D
 Acq: 11 Mar 2017 1:19

Instrument :
 BNA_G
 ClientSampleId :
 C0BF0

Tot Ion: 65 Resp: 2986
 Ion Ratio Lower Upper
 65 100
 92 0.0 60.4 90.6#
 138 0.0 99.8 149.6#

