





Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
Data File : BG026176.D
Acq On : 10 Mar 2017 16:45
Operator : SJ/MA
Sample : I2180-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 11 00:24:13 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 23:28:49 2017
Response via : Initial Calibration

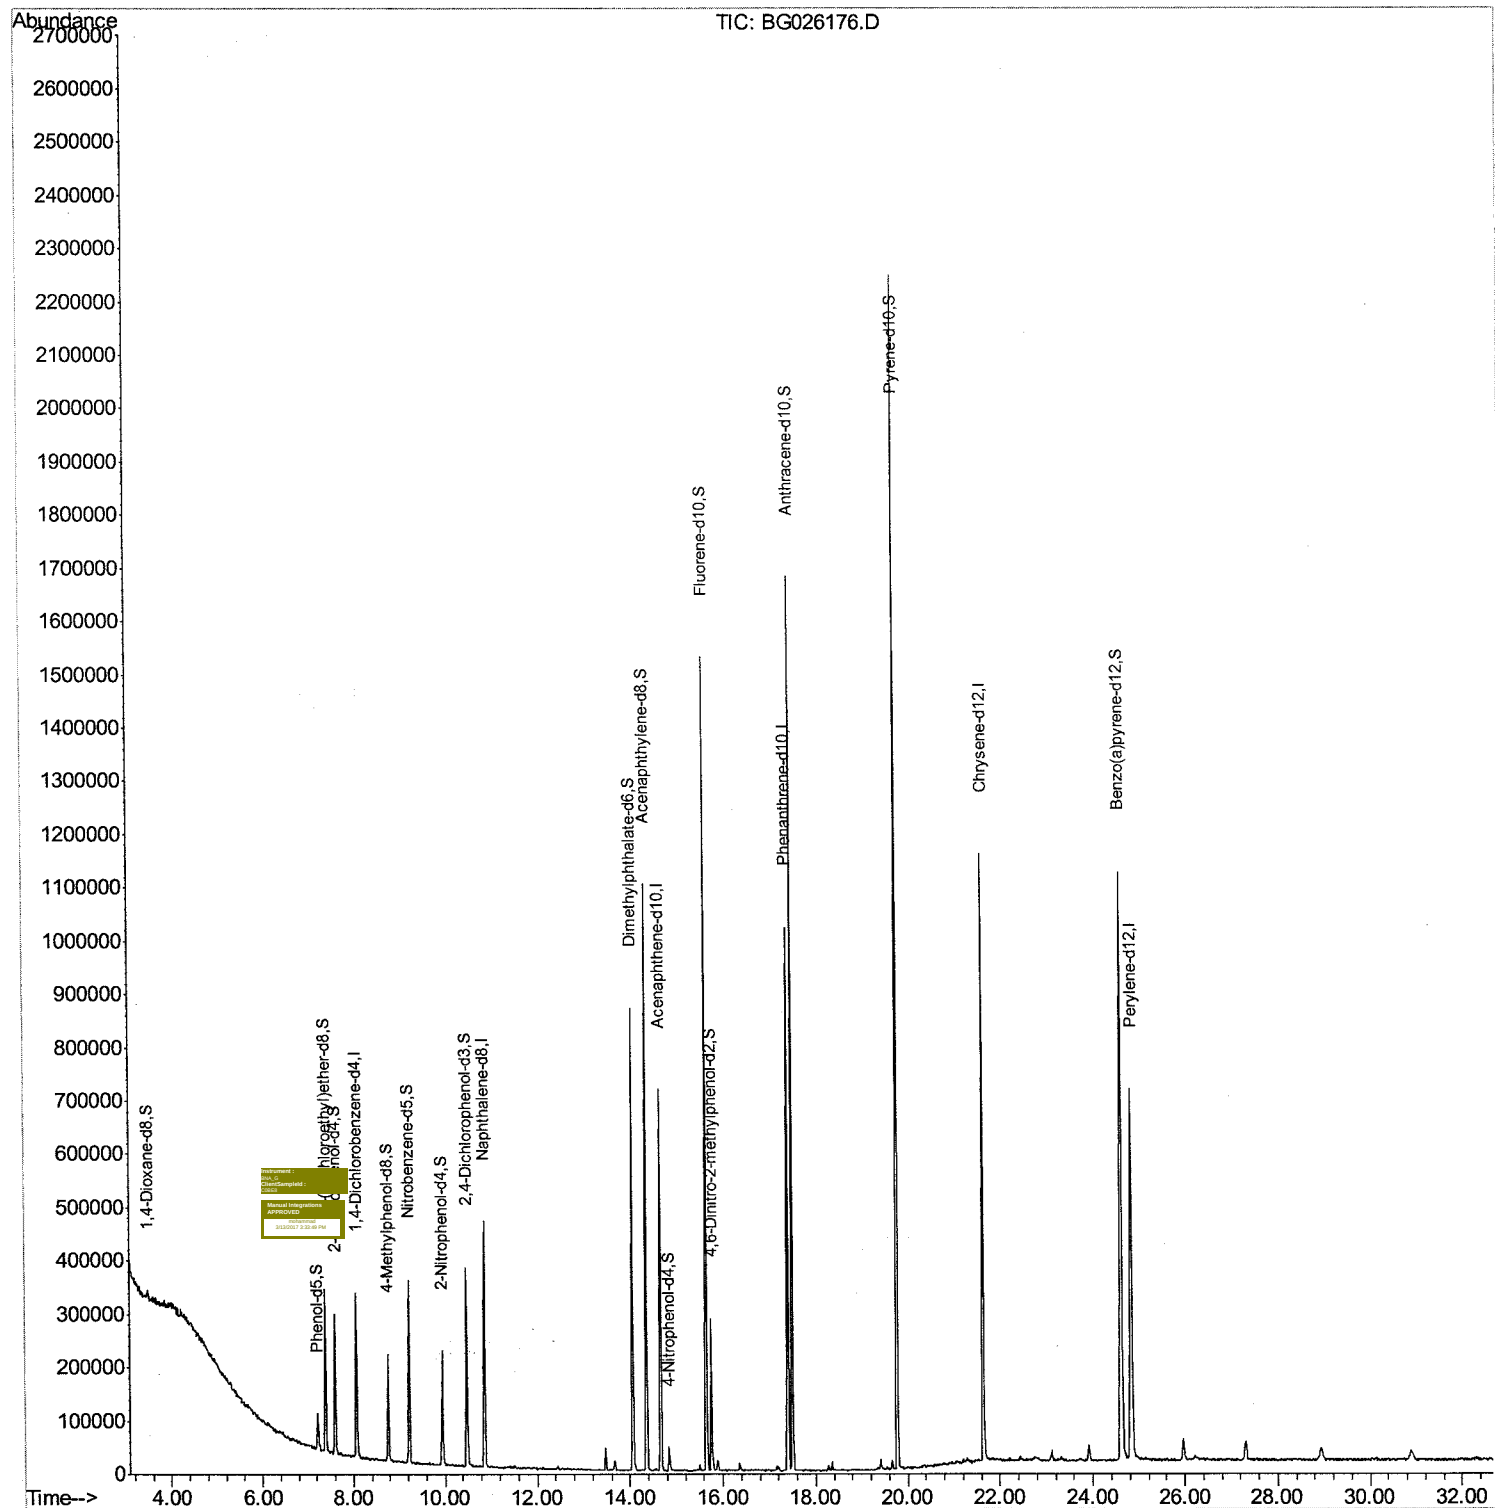

Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
 Data File : BG026176.D
 Acq On : 10 Mar 2017 16:45
 Operator : SJ/MA
 Sample : I2180-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 10 23:58:35 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 10 23:28:49 2017
 Response via : Initial Calibration

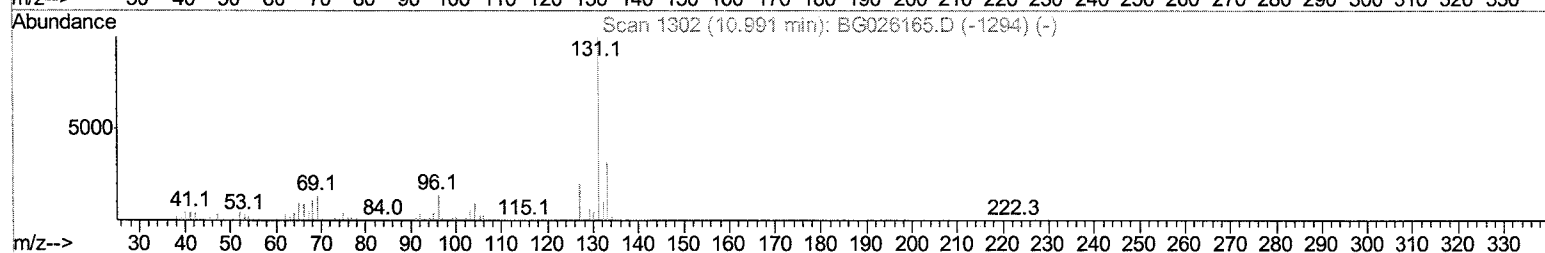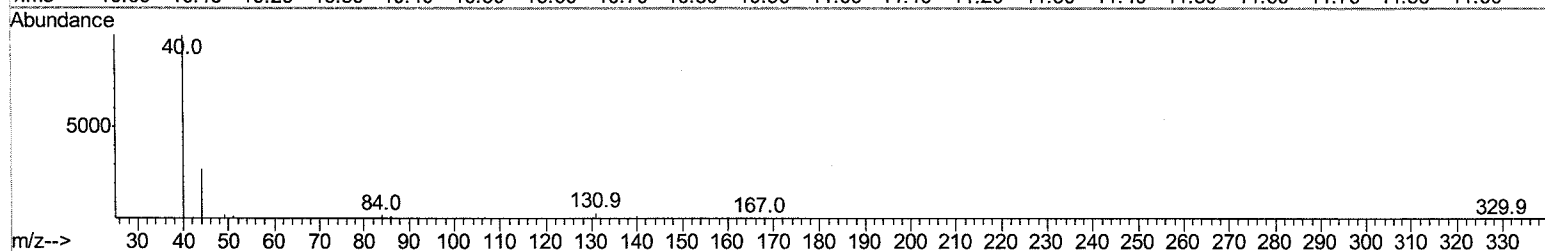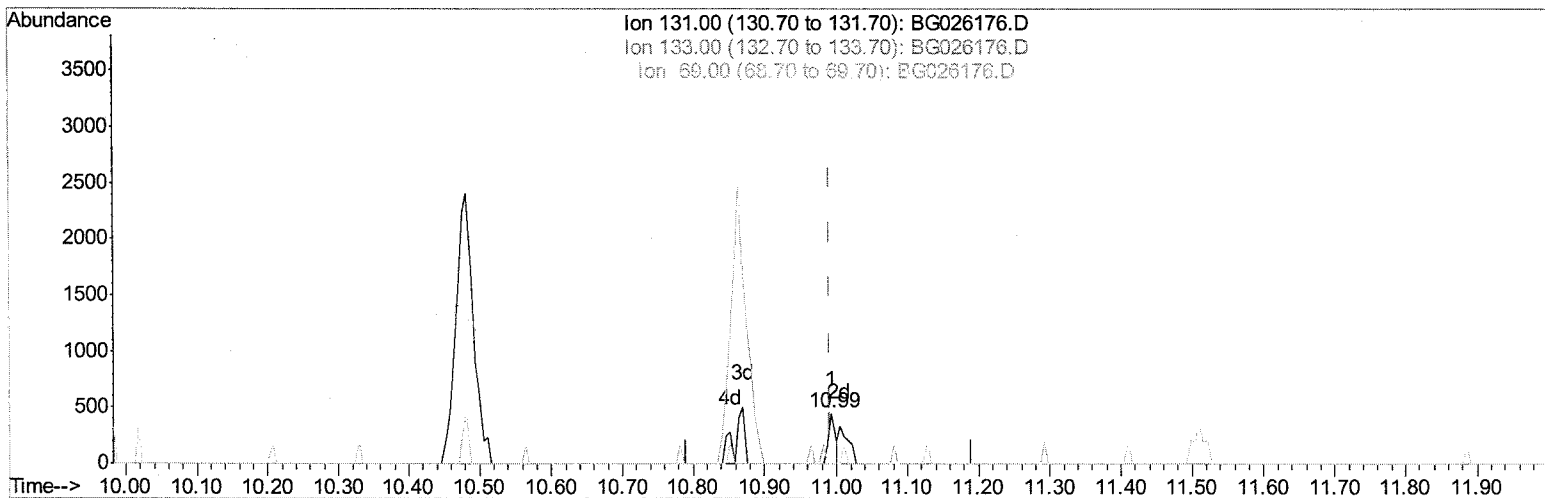

TIC: BG026176.D

(29) 4-Chloroaniline-d4 (S)

10.993min (+0.002) 0.04ng/ui




response 283

Ion	Exp%	Found%
131.00	100	100
133.00	32.10	0.00#
69.00	16.20	0.00#
0.00	0.00	0.00



Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
Data File : BG026176.D
Acq On : 10 Mar 2017 16:45
Operator : SJ/MA
Sample : I2180-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 10 23:58:35 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 10 23:28:49 2017
Response via : Initial Calibration

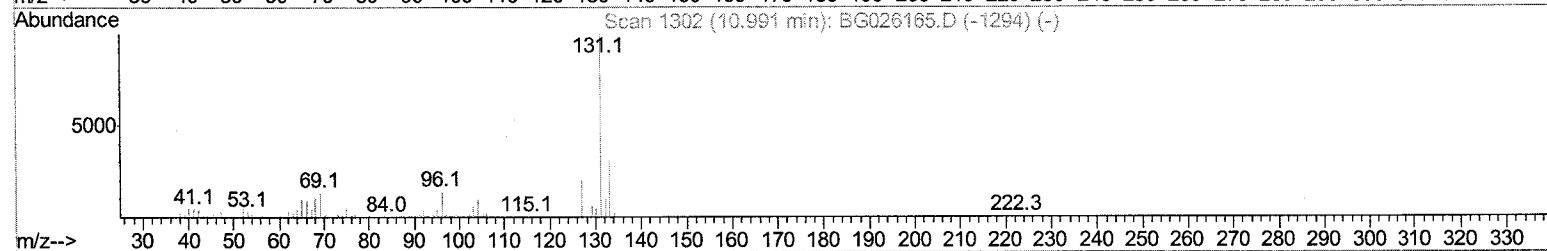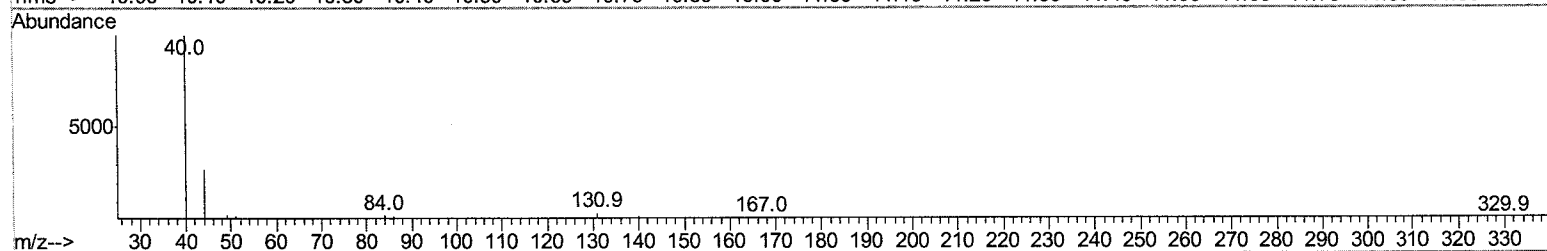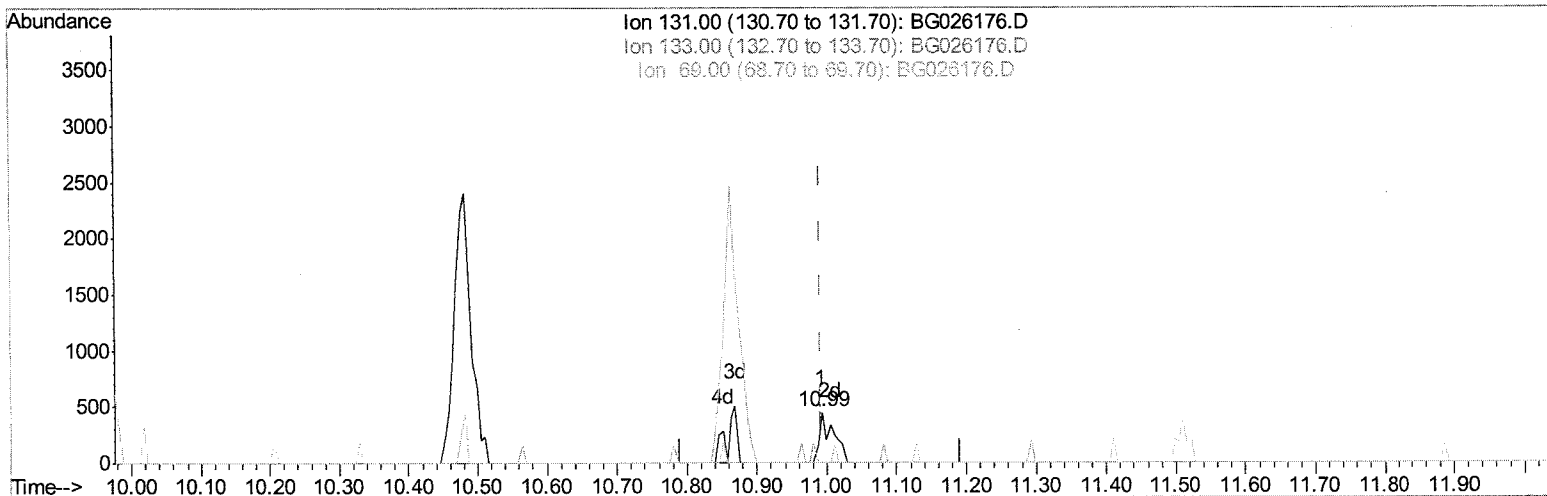

TIC: BG026176.D

(29) 4-Chloroaniline-d4 (S)

10.993min (+0.002) 0.08ng/ul m

SJ 3/13/17

response 622

Ion	Exp%	Manual Integration
131.00	100	100
133.00	32.10	0.00#
69.00	16.20	0.00#
0.00	0.00	0.00



Data Path : Z:\HPCHEM1\BNA G\DATA\BG031017\
 Data File : BG026176.D
 Acq On : 10 Mar 2017 16:45
 Operator : SJ/MA
 Sample : I2180-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Quant Time: Mar 11 00:24:13 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG030717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 10 23:28:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.07	152	98547	20.00	ng/ul	0.00
18) Naphthalene-d8	10.86	136	422075	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.67	164	249494	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.40	188	631365	20.00	ng/ul	0.00
77) Chrysene-d12	21.65	240	734558	20.00	ng/ul	0.00
85) Perylene-d12	24.84	264	708821	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	8390	3.66	ng/ul	0.00
5) Phenol-d5	7.22	99	44884	6.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.39	67	144849	31.32	ng/ul	0.00
9) 2-Chlorophenol-d4	7.60	132	147047	24.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	84053	14.68	ng/ul	0.00
19) Nitrobenzene-d5	9.22	128	102108	33.49	ng/ul	0.00
22) 2-Nitrophenol-d4	9.94	143	87906	35.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.48	165	167745	29.96	ng/ul	0.00
29) 4-Chloroaniline-d4	10.99	131	622m>	0.08	ng/ul	0.00
43) Dimethylphthalate-d6	14.07	166	623489	38.42	ng/ul	0.00
46) Acenaphthylene-d8	14.36	160	830456	38.12	ng/ul	0.00
51) 4-Nitrophenol-d4	14.85	143	14135	4.42	ng/ul	0.00
57) Fluorene-d10	15.65	176	613384	38.33	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.76	200	68548	23.14	ng/ul	0.00
70) Anthracene-d10	17.50	188	1001529	34.96	ng/ul	0.00
78) Pyrene-d10	19.77	212	1183879	39.18	ng/ul	0.00
89) Benzo(a)pyrene-d12	24.62	264	1085374	34.74	ng/ul	0.00

SJ 3/13/17

Target Compounds	Ovalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

